



Agilent Technologies
Innovating the HP Way

ENG#86

Service Guide



Agilent 34970A Data Acquisition / Switch Unit

Copyright © 1999
Hewlett-Packard Company
All Rights Reserved.

Printing History

Edition 1, June 1997
Edition 2, October 1997
Edition 3, November 1999

New editions are complete revisions of the manual. Update packages, which are issued between editions, may contain additional information and replacement pages which you merge into the manual. The dates on this page change only when a new edition is published.

Certification

Hewlett-Packard (HP) certifies that this product met its published specifications at the time of shipment. HP further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology (formerly National Bureau of Standards), to the extent allowed by that organization's calibration facility, and to the calibration facilities of other International Standards Organization members.

Warranty

This HP product is warranted against defects in materials and workmanship for a period of three years from date of shipment. Duration and conditions of warranty for this product may be superceded when the product is integrated into (becomes a part of) other HP products. During the warranty period, HP will, at its option, either repair or replace products which prove to be defective.

For warranty information on HP BenchLink Data Logger, refer to the on-line warranty statements.

Warranty Service

For warranty service or repair, this product must be returned to a service facility designated by HP. For products returned to HP for warranty service, the Buyer shall prepay shipping charges to HP and HP shall pay shipping charges to return the product to the Buyer. However, the Buyer shall pay all shipping charges, duties, and taxes for products returned to HP from another country.

Limitation of Warranty

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by the Buyer, Buyer-supplied products or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

The design and implementation of any circuit on this product is the sole responsibility of the Buyer.

HP does not warrant the Buyer's circuitry or malfunctions of HP products that result from the Buyer's circuitry. In addition, HP does not warrant any damage that occurs as a result of the Buyer's circuit or any defects that result from Buyer-supplied products.

HP makes no other warranty, expressed or implied, whether written or oral with respect to this product and specifically disclaims any implied warranty or condition of merchantability, fitness for a particular purpose or satisfactory quality.

Exclusive Remedies

The remedies provided herein are the Buyer's sole and exclusive remedies. HP shall not be liable for any direct, indirect, special, incidental, or consequential damages (including lost profit), whether based on warranty, contract, tort, or any other legal theory.

Notice

The information contained in this document is subject to change without notice.

Hewlett-Packard makes no warranty of any kind with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Hewlett-Packard shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material. No part of this document may be photocopied, reproduced, or translated to another language without the prior written consent of HP.

Restricted Rights

The Software and Documentation have been developed entirely at private expense. They are delivered and licensed as "commercial computer software" as defined in DFARS 252.227-7013 (Oct 1988), DFARS 252.211-7015 (May 1991), or DFARS 252.227-7014 (Jun 1995), as a "commercial item" as defined in FAR 2.101(a), or as "restricted computer software" as defined in FAR 52.227-19 (Jun 1987) (or any equivalent agency regulation or contract clause), whichever is applicable. You have only those rights provided for such Software and Documentation by the applicable FAR or DFARS clause or the HP standard software agreement for the product involved.

Trademark Information

Windows, Windows 95, and Windows NT are registered trademarks of Microsoft Corp.

Safety

Do not install substitute parts or perform any unauthorized modification to the product. Return the product to an HP Sales and Service Office for service and repair to ensure that safety features are maintained.

Safety Symbols

Warning

Calls attention to a procedure, practice, or condition, that could possibly cause bodily injury or death.

Caution

Calls attention to a procedure, practice, or condition that could possibly cause damage to equipment or permanent loss of data.



Earth ground symbol.



Chassis ground symbol.

Warning

Only qualified, service-trained personnel who are aware of the hazards involved should remove the cover from the instrument or connect external wiring to a plug-in module.

Warning

For continued protection against fire, replace the line fuse only with a fuse of the specified type and rating.

Contents

The Front Panel at a Glance	2
The Front-Panel Menus at a Glance	3
Display Annunciators	4
The Rear Panel at a Glance	5
The Plug-In Modules at a Glance	6
In This Book	9
Chapter 1 – Specifications	15
Chapter 2 – Quick Start	33
Chapter 3 – Menu Tutorial	47
Chapter 4 – Calibration Procedures	61
Chapter 5 – Theory of Operation	99
Chapter 6 – Service	139
Chapter 7 – Replaceable Parts	162
Chapter 8 – Backdating	199
Chapter 9 – Schematics	203

Factory Reset State

Specifications

Quick Start

The table below shows the state of the instrument after a **FACTORY RESET** from the **Sto/Rcl** menu or ***RST** command from the remote interface.

Front-Panel Overview

Calibration Procedures

Theory of Operation

Service

Replaceable Parts

Backdating

Schematics

Measurement Configuration	Factory Reset State
Function	DC Volts
Range	Autorange
Resolution	5½ digits
Integration Time	1 PLC
Input Resistance	10 M Ω (fixed for all DCV ranges)
Channel Delay	Automatic Delay
Totalizer Reset Mode	Count Not Reset When Read
Totalizer Edge Detect	Rising Edge
Scanning Operations	Factory Reset State
Scan List	Empty
Reading Memory	All Readings are Cleared
Min, Max, and Average	All Statistical Data is Cleared
Scan Interval Source	Immediate
Scan Interval	Front Panel = 10 Seconds
	Remote = Immediate
Scan Count	Front Panel = Continuous
	Remote = 1 Scan Sweep
Scan Reading Format	Reading Only (No Units, Channel, Time)
Monitor in Progress	Stopped
Mx+B Scaling	Factory Reset State
Gain Factor ("M")	1
Scale Factor ("B")	0
Scale Label	Vdc
Alarm Limits	Factory Reset State
Alarm Queue	Not Cleared
Alarm State	Off
HI and LO Alarm Limits	0
Alarm Output	Alarm 1
Alarm Output Configuration	Latched Mode
Alarm Output State	Output Lines are Cleared
Alarm Output Slope	Fail = Low
Module Hardware	Factory Reset State
34901A, 34902A, 34908A	Reset: All Channels Open
34903A, 34904A	Reset: All Channels Open
34905A, 34906A	Reset: Channels s11 and s21 Selected
34907A	Reset: Both DIO Ports = Input, Count = 0, Both DACs = 0 Vdc
System-Related Operations	Factory Reset State
Display State	On
Error Queue	Errors Not Cleared
Stored States	No Change

Note: *Unless otherwise indicated, this manual applies to all serial numbers.*

The Agilent Technologies 34970A combines precision measurement capability with flexible signal connections for your production and development test systems. Three module slots are built into the rear of the instrument to accept any combination of data acquisition or switching modules. The combination of data logging and data acquisition features makes this instrument a versatile solution for your testing requirements now and in the future.

Convenient Data Logging Features

- Direct measurement of thermocouples, RTDs, thermistors, dc voltage, ac voltage, resistance, dc current, ac current, frequency, and period
- Interval scanning with storage of up to 50,000 time-stamped readings
- Independent channel configuration with function, Mx+B scaling, and alarm limits available on a per-channel basis
- Intuitive user interface with knob for quick channel selection, menu navigation, and data entry from the front panel
- Portable, ruggedized case with non-skid feet
- *BenchLink Data Logger Software* for Microsoft® Windows® included


Flexible Data Acquisition/Switching Features

- 6½-digit multimeter accuracy, stability, and noise rejection
- Up to 60 channels per instrument (120 single-ended channels)
- Reading rates up to 600 readings per second on a single channel and scan rates up to 250 channels per second
- Choice of multiplexing, matrix, general-purpose Form C switching, RF switching, digital I/O, totalize, and 16-bit analog output functions
- GPIB (IEEE-488) interface and RS-232 interface are standard
- SCPI (*Standard Commands for Programmable Instruments*) compatibility

Agilent 34970A

Data Acquisition/Switch Unit

The Front Panel at a Glance

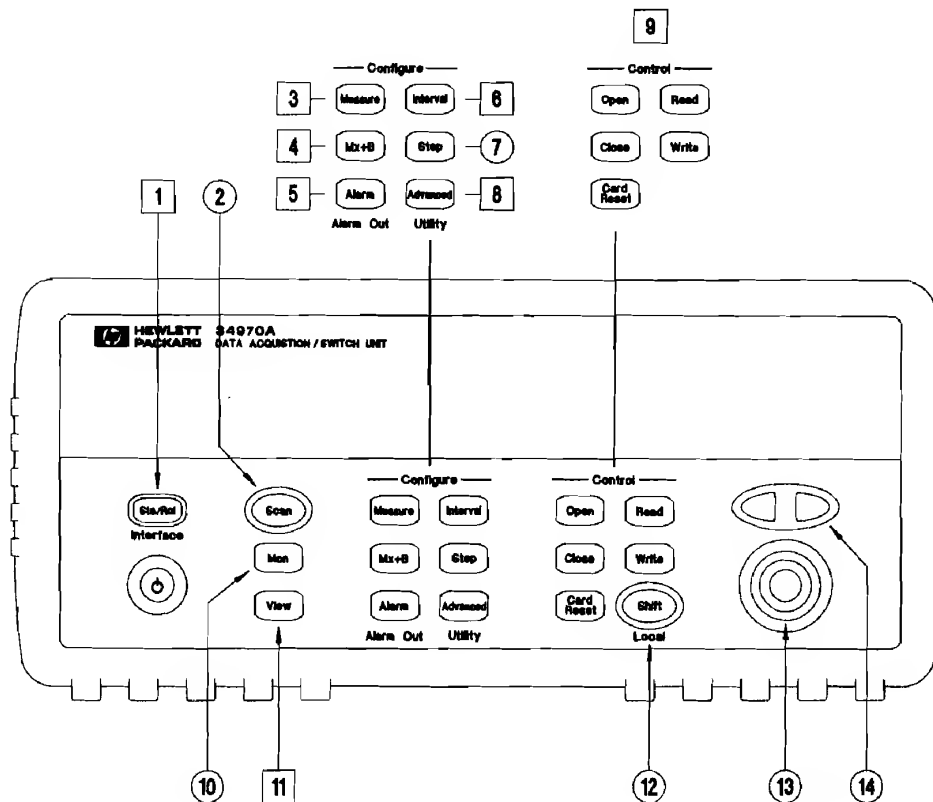


☐ Denotes a menu key. See the next page for details on menu operation.

- | | |
|---|---|
| 1 State Storage / Remote Interface Menus | 8 Advanced Measurement / Utility Menus |
| 2 Scan Start / Stop Key | 9 Low-Level Module Control Keys |
| 3 Measurement Configuration Menu | 10 Single-Channel Monitor On/Off Key |
| 4 Scaling Configuration Menu | 11 View Scanned Data, Alarms, Errors Menu |
| 5 Alarm / Alarm Output Configuration Menu | 12 Shift / Local Key |
| 6 Scan-to-Scan Interval Menu | 13 Knob |
| 7 Scan List Single Step/Read Key | 14 Navigation Arrow Keys |


The Front-Panel Menus at a Glance

Several of the front-panel keys guide you through menus to configure various parameters of the instrument (see previous page). The following steps demonstrate the menu structure using the **Sto/Rcl** key.

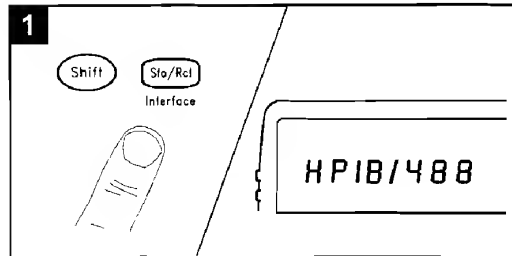


- 1 Press the menu key. You are automatically guided to the first level of the menu. Rotate the knob to view the other choices on the first level of the menu.

The menu will automatically timeout after about 20 seconds of inactivity. You will be returned to the operation in progress prior to entering the menu.

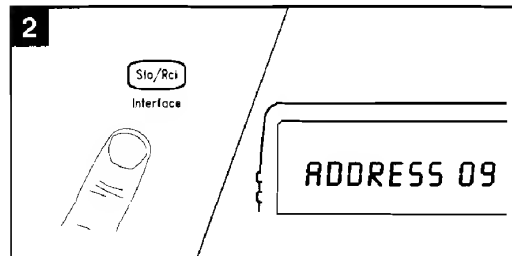


- 2 Press the *same* menu key again to move to the next item of the menu. Typically, this is where you choose parameter values for the selected operation.

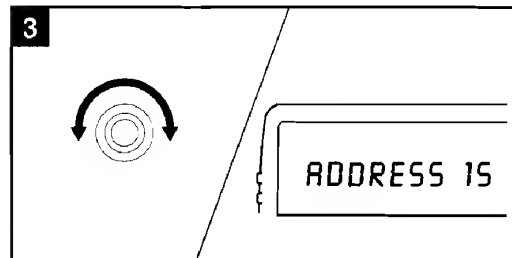

- 3 Rotate the knob to view the choices on this level of the menu. When you reach the end of the list, rotate the knob in the opposite direction to view all of the other choices.


The current selection is highlighted for emphasis. All other choices are dimmed.

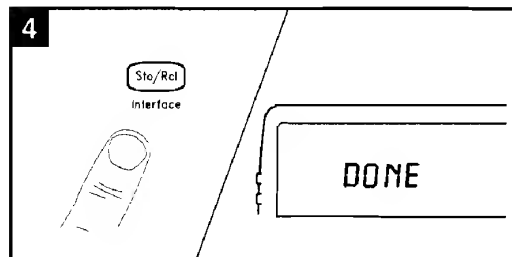

- 4 Press the *same* menu key again to accept the change and exit the menu. A brief confirmation message is displayed.

Tip: To review the current configuration of a specific menu, press the menu key several times. A message **NO CHANGES** is displayed when you exit the menu.


Display Annunciators

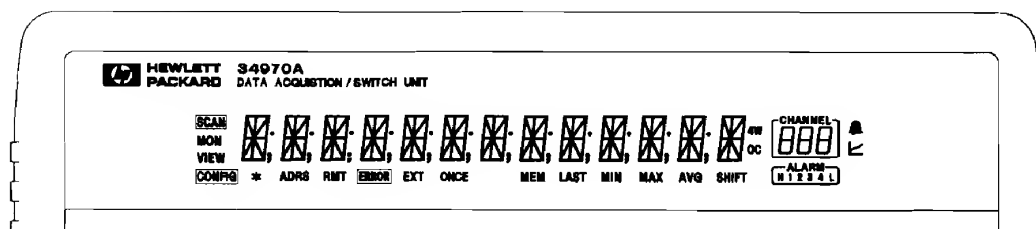

SCAN	Scan is in progress or enabled. <i>Press and hold Scan again to turn off.</i>
MON	Monitor mode is enabled. <i>Press Mon again to turn off.</i>
VIEW	Scanned readings, alarms, errors, or relay cycles are being viewed.
CONFIG	Channel configuration is in progress on displayed channel.
*	Measurement is in progress.
ADRS	Instrument is addressed to listen or talk over the remote interface.
RMT	Instrument is in remote mode (remote interface).
ERROR	Hardware or remote interface errors are detected. <i>Press View to read errors.</i>
EXT	Instrument is configured for an external scan interval.
ONCE	Scan Once mode is enabled. <i>Press Scan to initiate and hold key to disable.</i>
MEM	Reading memory overflow; new readings will overwrite the oldest readings.
LAST	Viewed data is the <i>last</i> reading stored during most recent scan.
MIN	Viewed data is the <i>minimum</i> reading stored during most recent scan.
MAX	Viewed data is the <i>maximum</i> reading stored during most recent scan.
SHIFT	Shift has been pressed. <i>Press Shift again to turn off.</i>
4W	4-wire function is in use on displayed channel.
OC	Offset compensation is enabled on displayed channel.
	Alarms are enabled on displayed channel.
	Mx+B scaling is enabled on displayed channel.
	HI or LO alarm condition has occurred on indicated alarms.

*To review the display annunciators, hold down the **Shift** key as you turn on the instrument.*

The Rear Panel at a Glance

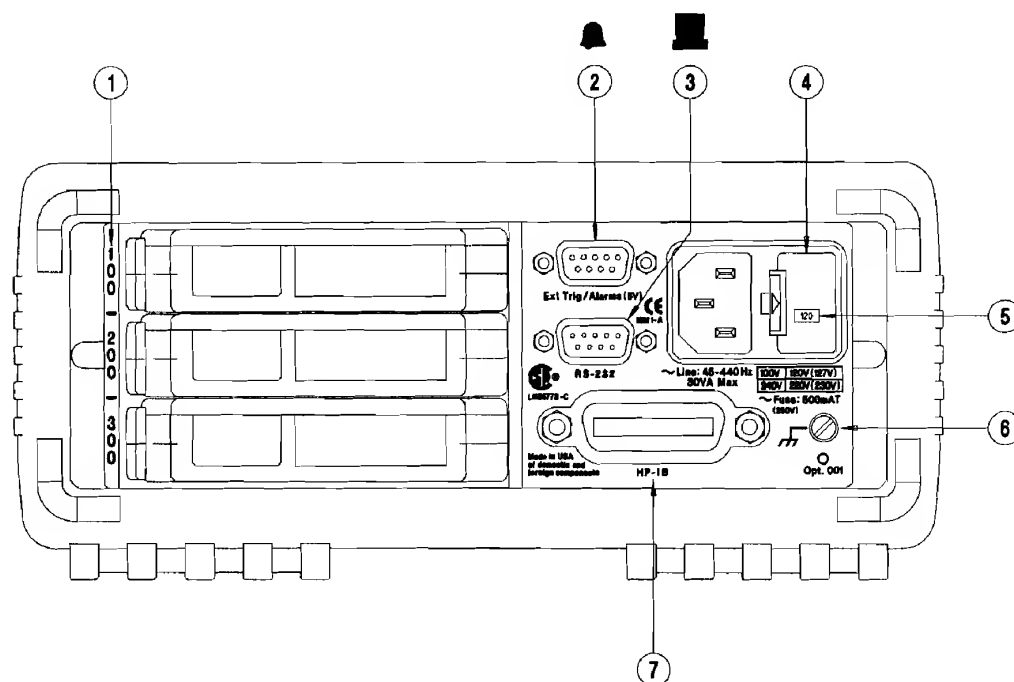

- | | |
|--|--|
| 1 Slot Identifier (100, 200, 300) | 4 Power-Line Fuse-Holder Assembly |
| 2 Ext Trig Input / Alarm Outputs / Channel Advance Input / Channel Closed Output | 5 Power-Line Voltage Setting |
| 3 RS-232 Interface Connector | 6 Chassis Ground |
| | 7 HP-IB (IEEE-488) Interface Connector |

Use the **Interface** Menu to:

- Select the HP-IB or RS-232 interface.
- Set the HP-IB address.
- Set the RS-232 baud rate, parity, and flow control mode.

WARNING

For protection from electrical shock, the power cord ground must not be defeated. If only a two-contact electrical outlet is available, connect the instrument's chassis ground screw (see above) to a good earth ground.

The Plug-In Modules at a Glance

For complete specifications on each plug-in module, refer to the module sections in chapter 1.



HP 34901A 20-Channel Armature Multiplexer

- 20 channels of 300 V switching
- Two channels for DC or AC current measurements (100 nA to 1 A)
- Built-in thermocouple reference junction
- Switching speed of up to 60 channels per second
- Connects to the internal multimeter

Each of the 20 channels switches both HI and LO inputs, thus providing fully isolated inputs to the internal multimeter. The module is divided into two banks of 10 two-wire channels each. When making four-wire resistance measurements, channels from *Bank A* are automatically paired with channels from *Bank B*. Two additional fused channels are included on the module (22 channels total) for making calibrated DC or AC current measurements with the internal multimeter (external shunt resistors are not required). You can close multiple channels on this module *only* if you have not configured any channels to be part of the scan list. Otherwise, all channels on the module are break-before-make.



HP 34902A 16-Channel Reed Multiplexer

- 16 channels of 300 V switching
- Built-in thermocouple reference junction
- Switching speed of up to 250 channels per second
- Connects to the internal multimeter


Use this module for high-speed scanning and high-throughput automated test applications. Each of the 16 channels switches both HI and LO inputs, thus providing fully isolated inputs to the internal multimeter. The module is divided into two banks of eight two-wire channels each. When making four-wire resistance measurements, channels from *Bank A* are automatically paired with channels from *Bank B*. You can close multiple channels on this module *only* if you have not configured any channels to be part of the scan list. Otherwise, all channels on the module are break-before-make.



HP 34903A 20-Channel Actuator/General-Purpose Switch

- 300 V, 2 A actuation and switching
- SPDT (Form C) latching relays
- Breadboard area for custom circuits

Use this module for those applications that require high-integrity contacts or quality connections of non-multiplexed signals. This module can switch 300 V, 1 A (50 W maximum switch power) to your device under test or to actuate external devices. Screw terminals on the module provide access to the Normally-Open, Normally-Closed, and Common contacts for each of the 20 switches. A breadboard area is provided near the screw terminals to implement custom circuitry, such as simple filters, snubbers, or voltage dividers.



HP 34904A 4x8 Two-Wire Matrix Switch

- 32 two-wire crosspoints
- Any combination of inputs and outputs can be connected at a time
- 300 V, 1 A switching


Use this module to connect multiple instruments to multiple points on your device under test at the same time. You can connect rows and columns between multiple modules to build larger matrices such as 8x8 and 4x16, with up to 96 crosspoints in a single mainframe.



HP 34905/6A Dual 4-Channel RF Multiplexers

- HP 34905A (50 Ω) / 34906A (75 Ω)
- 2 GHz bandwidth with on-board SMB connections
- 1 GHz bandwidth with SMB-to-BNC adapter cables provided

These modules offer wideband switching capabilities for high frequency and pulsed signals. Each module is organized in two independent banks of 4-to-1 multiplexers. Both modules offer low crosstalk and excellent insertion loss performance. To create larger RF multiplexers, you can cascade multiple banks together. Only one channel in each bank may be closed at a time.



HP 34907A Multifunction Module

- Two 8-bit Digital Input/Output ports, 400 mA sink, 42 V open collector
- 100 kHz Totalize input with 28 bits of resolution
- Two 16-bit, ± 12 V Calibrated Analog Outputs

Use this module to sense status and control external devices such as solenoids, power relays, and microwave switches. For greater flexibility, you can read digital inputs and the count on the totalizer during a scan.



HP 34908A 40-Channel Single-Ended Multiplexer

- 40 channels of 300 V single-ended (common LO) switching
- Built-in thermocouple isothermal reference junction
- Switching speed of up to 60 channels per second
- Connects to the internal multimeter

Use this module for high-density switching applications which require single-wire inputs with a common LO. All relays are break-before-make to ensure that only one relay is connected at any time.

In This Book

Specifications Chapter 1 lists the instrument's specifications and describes how to interpret these specifications.

Quick Start Chapter 2 prepares the instrument for use and helps you get familiar with a few of its front-panel features.

Menu Tutorial Chapter 3 introduces you to the front-panel menu and describes some of the instrument's menu features.

Calibration Procedures Chapter 4 provides calibration, verification, and adjustment procedures for the instrument.

Theory of Operation Chapter 5 describes block and circuit level theory related to the operation the instrument.

Service Chapter 6 provides guidelines for returning your instrument to Hewlett-Packard for servicing, or for servicing it yourself.

Replaceable Parts Chapter 7 contains a detailed parts lists of the instrument.

Backdating Chapter 8 describes the differences between this manual and older issues of this manual.

Schematics Chapter 9 contains the instrument's block diagram, schematics, disassembly drawings, and component locator drawings.



*If you have questions relating to the operation of the HP 34970A, call **1-800-452-4844** in the United States, or contact your nearest Hewlett-Packard Sales Office.*

*If your HP 34970A fails within three years of original purchase, we will repair or replace it free of charge. Call **1-800-258-5165** and ask for "Express Exchange."*

Contents

Chapter 1 Specifications

- To Calculate Total Measurement Error, 26
- Interpreting Internal DMM Specifications, 28
 - Number of Digits and Overrange, 28
 - Sensitivity, 28
 - Resolution, 29
 - Accuracy, 29
 - 24-Hour Accuracy, 30
 - 90-Day and 1-Year Accuracy, 30
 - Temperature Coefficients, 30
- Configuring for Highest Accuracy Measurements, 31

Chapter 2 Quick Start

- To Prepare the Instrument for Use, 35
- To Connect Wiring to a Module, 36
- To Set the Time and Date, 38
- To Configure a Measurement Channel, 39
- To Monitor a Single Channel, 40
- To Close a Channel, 41
- If the Instrument Does Not Turn On, 42
- To Adjust the Carrying Handle, 44
- To Rack Mount the Instrument, 45

Chapter 3 Front-Panel Overview

- Front-Panel Menu Reference, 49
- To Unsecure for Calibration, 51
- To Secure Against Calibration, 51
- To Change the Security Code, 52
- Error Messages, 52
- To Perform a Zero Adjustment, 53
- To Apply $Mx+B$ Scaling to Measurements, 54
- To Read the Relay Cycle Count, 55
- To Read a Digital Input Port, 56
- To Write to a Digital Output Port, 57
- To Read the Totalizer Count, 58
- To Output a DC Voltage, 59

Contents

Chapter 4 Calibration Procedures

- Hewlett-Packard Calibration Services, 63
- Calibration Interval, 63
 - Adjustment is recommended, 63
- Time Required for Calibration, 64
- Automating Calibration Procedures, 64
- Recommended Test Equipment, 65
- Input Connections, 66
- Calibration Security, 67
 - To Unsecure the Instrument Without the Security Code, 68
- Calibration Message, 69
- Calibration Count, 69
- Calibration Procedure, 70
- Aborting a Calibration in Progress, 70
- Test Considerations, 71
- Performance Verification Tests, 72
 - Self-Test, 73
 - Quick Performance Check, 74
 - Performance Verification Tests, 74
- Internal DMM Verification Tests, 75
 - Zero Offset Verification, 75
 - Gain Verification, 77
- Optional AC Performance Verification Tests, 80
- Internal DMM Adjustments, 81
 - Zero Adjustment, 81
 - Gain Adjustment, 82
- 10 Vdc Adjustment Procedure (Optional), 85
- Plug-in Module Test Considerations, 87
- Relay Verification, 88
- Relay Cycle Count, 88
 - HP 34901A Relay Contact Resistance Verification (Optional), 89
 - HP 34902A Relay Contact Resistance Verification (Optional), 90
 - HP 34903A Relay Contact Resistance Verification (Optional), 91
 - HP 34904A Relay Contact Resistance Verification (Optional), 92
 - HP 34905A/06A Relay Contact Resistance Verification (Optional), 92
 - HP 34908A Relay Contact Resistance Verification (Optional), 93
- Thermocouple Reference Junction (Optional), 94
 - Thermocouple Reference Junction Verification, 94
 - Thermocouple Reference Junction Adjustments, 95
- HP 34907A Analog Output, 96
 - Analog Output Verification Test, 96
 - Analog Output Adjustment, 97

Contents

Chapter 5 Theory of Operation

System Block Diagram, 101
Floating Logic, 102
Memory, 105
Earth-Referenced Logic, 106
Power Supplies, 107
Front Panel, 109
Backplane, 110
Analog Bus, 110
Digital Bus, 110
Internal DMM, 111
DMM Block Diagram , 111
Input, 112
Input Amplifier, 113
Ohms Current Source , 115
AC Circuit , 116
A-to-D Converter, 118
Switch Modules, 120
Switch Module Control, 120
Relay Drivers, 122
HP 34901A, 124
HP 34902A, 126
HP 34903A, 128
HP 34904A, 129
HP 34905A/34906A, 129
HP 34908A , 131
Multifunction Module, 133
Multifunction Control, 133
Totalizer, 135
Analog Output, 136
Digital I/O, 137

Chapter 6 Service

Operating Checklist, 141
Is the instrument inoperative?, 141
Does the instrument fail self-test?, 141
Is the Current Measurement Function Inoperative?, 141
Types of Service Available, 142
Standard Repair Service (worldwide), 142
Express Exchange (U.S.A. only), 142
Repackaging for Shipment, 143
Electrostatic Discharge (ESD) Precautions, 144
Surface Mount Repair, 144
To Replace the Power-Line Fuse, 144

Contents

Chapter 6 Service (continued)

- Troubleshooting Hints, 145
 - Unit is inoperative, 145
 - Unit reports error 705, 146
 - Isolating to an Assembly, 146
 - Unit fails self-test, 146
 - Power supplies, 147
- Self-Test Procedures, 149
 - Power-On Self-Test, 149
 - Complete Self-Test, 149
 - Plug-in Module Self-Test, 149
 - Self-Tests, 150
- Battery Check and Replacement, 154
 - To verify the battery:, 155
 - To replace the battery:, 155
- Disassembly, 156
 - General Disassembly, 157
 - Internal DMM Disassembly, 158
 - Front Panel Disassembly, 159
 - Additional Disassembly, 160
 - Plug-in Module Disassembly, 161

Chapter 7 Replaceable Parts

- Replaceable Parts, 164
 - To Order Replace Parts, 164
 - Backdating and Part Changes, 164
 - HP 34970 Mainframe, 165
 - 34970-66501 A1 PC Assembly, 166
 - 34970-66502 A2 PC Assembly, 171
 - 34970-66503 A3 PC Assembly, 172
 - 34970-66504 A4 PC Assembly, 173
 - HP 34901A 20-Channel Multiplexer, 178
 - HP 34902A 16-Channel Multiplexer, 181
 - HP 34903A 20-Channel Actuator Rev B, 183
 - HP 34904A 4x8 Matrix, 185
 - HP 34905A/34906A RF Multiplexer, 188
 - HP 34907A Multifunction Module, 190
 - HP 34908A 40-Channel Multiplexer, 194
 - Manufacturer's List, 197

Chapter 8 Backdating

- HP 34903A 20-Channel Actuator Rev A, 200

Contents

Chapter 9 Schematics

HP 34970A System Block Diagram,	205
A1 Component Locator (<i>top</i>),	206
A1 Component Locator (<i>bottom</i>),	207
A1 Power Supply Schematic <i>Sheet 1 of 4</i> ,	208
A1 Floating Logic Schematic <i>Sheet 2 of 4</i> ,	209
A1 Earth Referenced Logic Schematic <i>Sheet 3 of 4</i> ,	210
A1 Memory Schematic <i>Sheet 4 of 4</i> ,	211
A2 Component Locator,	212
A2 Display and Keyboard Schematic,	213
A3 Component Locator,	214
A3 Backplane Schematic,	215
A4 Component Locator (<i>top</i>),	216
A4 Component Locator (<i>bottom</i>),	217
A4 Input and Protection Schematic <i>Sheet 1 of 4</i> ,	218
A4 Input Amplifier and Ohms Current Schematic <i>Sheet 2 of 4</i> ,	219
A4 AC Schematic <i>Sheet 3 of 4</i> ,	220
A4 A/D Converter Schematic <i>Sheet 4 of 4</i> ,	221
HP 34901A 20-Channel Multiplexer Component Locator,	222
HP 34901A 20-Channel Multiplexer Schematic <i>Sheet 1 of 5</i> ,	223
HP 34901A 20-Channel Multiplexer Schematic <i>Sheet 2 of 5</i> ,	224
HP 34901A 20-Channel Multiplexer Schematic <i>Sheet 3 of 5</i> ,	225
HP 34901A 20-Channel Multiplexer Schematic <i>Sheet 4 of 5</i> ,	226
HP 34901A 20-Channel Multiplexer Schematic <i>Sheet 5 of 5</i> ,	227
HP 34902A 16-Channel Multiplexer Component Locator,	228
HP 34902A 16-Channel Multiplexer Schematic <i>Sheet 1 of 4</i> ,	229
HP 34902A 16-Channel Multiplexer Schematic <i>Sheet 2 of 4</i> ,	230
HP 34902A 16-Channel Multiplexer Schematic <i>Sheet 3 of 4</i> ,	231
HP 34902A 16-Channel Multiplexer Schematic <i>Sheet 4 of 4</i> ,	232
HP 34903A 20-Channel Actuator Component Locator,	233
HP 34903A 20-Channel Actuator Schematic <i>Sheet 1 of 3</i> ,	234
HP 34903A 20-Channel Actuator Schematic <i>Sheet 2 of 3</i> ,	235
HP 34903A 20-Channel Actuator Schematic <i>Sheet 3 of 3</i> ,	236
HP 34904A 4x8 Matrix Component Locator,	237
HP 34904A 4x8 Matrix Schematic <i>Sheet 1 of 3</i> ,	238
HP 34904A 4x8 Matrix Schematic <i>Sheet 2 of 3</i> ,	239
HP 34904A 4x8 Matrix Schematic <i>Sheet 3 of 3</i> ,	240
HP 34905A/34906A RF Multiplexer Component Locator,	241
HP 34905A/34906A RF Multiplexer Schematic <i>Sheet 1 of 2</i> ,	242
HP 34905A/34906A RF Multiplexer Schematic <i>Sheet 2 of 2</i> ,	243
HP 34907A Multifunction Module Component Locator,	244
HP 34907A Multifunction Module Schematic <i>Sheet 1 of 5</i> ,	245
HP 34907A Multifunction Module Schematic <i>Sheet 2 of 5</i> ,	246
HP 34907A Multifunction Module Schematic <i>Sheet 3 of 5</i> ,	247
HP 34907A Multifunction Module Schematic <i>Sheet 4 of 5</i> ,	248
HP 34907A Multifunction Module Schematic <i>Sheet 5 of 5</i> ,	249
HP 34908A 40-Channel Multiplexer Component Locator,	250
HP 34908A 40-Channel Multiplexer Schematic <i>Sheet 1 of 3</i> ,	251
HP 34908A 40-Channel Multiplexer Schematic <i>Sheet 2 of 3</i> ,	252
HP 34908A 40-Channel Multiplexer Schematic <i>Sheet 3 of 3</i> ,	253

- DC, Resistance, and Temperature Accuracy Specifications, *on page 16*
- DC Measurement and Operating Characteristics, *on page 17*
- AC Accuracy Specifications, *on page 18*
- AC Measurement and Operating Characteristics, *on page 19*
- Measurement Rates and System Characteristics, *on page 20*
- Module Specifications:
 - HP 34901A, 34902A, 34908A, 34903A, 34904A, *on page 21*
 - HP 34905A, 34906A, *on page 22*
 - Typical AC Performance Graphs, *on page 23*
 - HP 34907A, *on page 24*
- HP BenchLink Data Logger Software Specifications, *on page 24*
- Product and Module Dimensions, *on page 25*
- To Calculate Total Measurement Error, *on page 26*
- Interpreting Multimeter Specifications, *on page 28*
- Configuring for Highest Accuracy Measurements, *on page 31*

Specifications

Chapter 1 Specifications
DC, Resistance, and Temperature Accuracy Specifications

■ DC, Resistance, and Temperature Accuracy Specifications

\pm (% of reading + % of range)^[1]

Includes measurement error, switching error, and transducer conversion error

Function	Range ^[3]	Test Current or Burden Voltage	24 Hour ^[2] 23 °C \pm 1 °C	90 Day 23 °C \pm 5 °C	1 Year 23 °C \pm 5 °C	Temperature Coefficient /°C 0 °C – 18 °C 28 °C – 55 °C
DC Voltage	100.0000 mV		0.0030 + 0.0035	0.0040 + 0.0040	0.0050 + 0.0040	0.0005 + 0.0005
	1.000000 V		0.0020 + 0.0006	0.0030 + 0.0007	0.0040 + 0.0007	0.0005 + 0.0001
	10.00000 V		0.0015 + 0.0004	0.0020 + 0.0005	0.0035 + 0.0005	0.0005 + 0.0001
	100.0000 V		0.0020 + 0.0006	0.0035 + 0.0006	0.0045 + 0.0006	0.0005 + 0.0001
	300.000 V		0.0020 + 0.0020	0.0035 + 0.0030	0.0045 + 0.0030	0.0005 + 0.0003
Resistance^[4]	100.0000 Ω	1 mA current source	0.0030 + 0.0035	0.008 + 0.004	0.010 + 0.004	0.0006 + 0.0005
	1.000000 k Ω	1 mA	0.0020 + 0.0006	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	10.00000 k Ω	100 μ A	0.0020 + 0.0005	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	100.0000 k Ω	10 μ A	0.0020 + 0.0005	0.008 + 0.001	0.010 + 0.001	0.0006 + 0.0001
	1.000000 M Ω	5 μ A	0.002 + 0.001	0.008 + 0.001	0.010 + 0.001	0.0010 + 0.0002
	10.00000 M Ω	500 nA	0.015 + 0.001	0.020 + 0.001	0.040 + 0.001	0.0030 + 0.0004
	100.0000 M Ω	500 nA // 10 M Ω	0.300 + 0.010	0.800 + 0.010	0.800 + 0.010	0.1500 + 0.0002
DC Current <i>HP 34901A Only</i>	10.00000 mA	< 0.1 V burden	0.005 + 0.010	0.030 + 0.020	0.050 + 0.020	0.002 + 0.0020
	100.0000 mA	< 0.6 V	0.010 + 0.004	0.030 + 0.005	0.050 + 0.005	0.002 + 0.0005
	1.000000 A	< 2 V	0.050 + 0.006	0.080 + 0.010	0.100 + 0.010	0.005 + 0.0010
Temperature	Type	Best Range Accuracy ^[5]		Extended Range Accuracy ^[5]		
Thermocouple	B	1100°C to 1820°C	1.2°C	400°C to 1100°C	1.8°C	0.03°C
	E	-150°C to 1000°C	1.0°C	-260°C to -150°C	1.5°C	0.03°C
	J	-150°C to 1200°C	1.0°C	-210°C to -150°C	1.2°C	0.03°C
	K	-100°C to 600°C	1.0°C	-230°C to -100°C	1.5°C	0.03°C
	N	-100°C to 1300°C	1.0°C	-220°C to -100°C	1.5°C	0.03°C
	R	300°C to 1760°C	1.2°C	-50°C to 300°C	1.8°C	0.03°C
	S	400°C to 1760°C	1.2°C	-50°C to 400°C	1.8°C	0.03°C
	T	-100°C to 400°C	1.0°C	-240°C to -100°C	1.5°C	0.03°C
RTD	R ₀ from 49 Ω to 2.1 k Ω	-200°C to 600°C	0.06°C			0.003°C
Thermistor	2.2 k, 5 k, 10 k	-80°C to 150°C	0.08°C			0.002°C

[1] Specifications are for 1 hour warm up and 6½ digits

[2] Relative to calibration standards

[3] 20% over range on all ranges except 300 Vdc and 1 Adc ranges

[4] Specifications are for 4-wire ohms function or 2-wire ohms using Scaling to remove the offset.
Without Scaling, add 1 Ω additional error in 2-wire ohms function.

[5] 1 year accuracy. For total measurement accuracy, add temperature probe error.

■ DC Measurement and Operating Characteristics

DC Measurement Characteristics ^[1]

DC Voltage	
Measurement Method:	Continuously Integrating, Multi-slope III A/D Converter
A/D Linearity:	0.0002% of reading + 0.0001% of range
Input Resistance:	100 mV, 1 V, 10 V ranges: Selectable 10 MΩ or > 10 GΩ
	100 V, 300 V ranges: 10 MΩ ±1%
Input Bias Current:	< 30 pA at 25 °C
Input Protection:	300 V on all ranges
Resistance	
Measurement Method:	Selectable 4-wire or 2-wire Ohms, Current source reference to LO input
Offset Compensation:	Selectable on 100Ω, 1 kΩ, 10 kΩ ranges
Max. Lead Resistance:	10% of range per lead for 100Ω and 1 kΩ ranges. 1 kΩ on all other ranges
Input Protection:	300 V on all ranges
DC Current	
Shunt Resistance:	5Ω for 10 mA, 100 mA; 0.1Ω for 1A.
Input Protection:	1.5A 250 V fuse on HP 34901A module
Thermocouple	
Conversion:	ITS-90 software compensation
Reference Junction Type:	Internal, Fixed, or External
Open T/C Check:	Selectable per channel. Open > 5 kΩ
RTD	$\alpha = 0.00385$ (DIN) and 0.00392
Thermistor	44004, 44007, 44006 series
Measurement Noise Rejection 60 Hz (50 Hz) ^[2]	
DC CMRR:	140 dB
Integration Time	
200 PLC / 3.33s (4s)	110 dB ^[4]
100 PLC / 1.67s (2s)	105 dB ^[4]
20 PLC / 333 ms (400 ms)	100 dB ^[4]
10 PLC / 167 ms (200 ms)	95 dB ^[4]
2 PLC / 33.3 ms (40 ms)	90 dB
1 PLC / 16.7 ms (20 ms)	60 dB
< 1 PLC	0 dB
Normal Mode Rejection ^[3]	

DC Operating Characteristics ^[5]

Function	Digits ^[6]	Readings/s	Additional Noise Error
DCV, DCI, and Resistance:	6½	0.6 (0.5)	0% of range
	6½	6 (5)	0% of range
	5½	60 (50)	0.001% of range
	5½	300	0.001% of range ^[7]
	4½	600	0.01% of range ^[7]

Single Channel Measurement Rates ^[8]			
Function	Resolution	Readings/s	
DCV, 2-Wire Ohms:	6½ (10 PLC)	6 (5)	
	5½ (1 PLC)	57 (47)	
	4½ (0.02 PLC)	600	
Thermocouple:	0.1 °C (1 PLC)	57 (47)	
	(0.02 PLC)	220	
RTD, Thermistor:	0.01 °C (10 PLC)	6 (5)	
	0.1 °C (1 PLC)	57 (47)	
	1 °C (0.02 PLC)	220	

Autozero OFF Operation
Following instrument warm-up at calibration temperature ±1 °C and < 10 minutes, add 0.0002% range additional error + 5 μV.

Settling Considerations
Reading settling times are affected by source impedance, low dielectric absorption characteristics, and input signal changes.

[1] 300 Vdc isolation voltage (ch-ch, ch-earth)
[2] For 1 kΩ unbalance in LO lead
[3] For power line frequency ±0.1%
[4] For power line frequency ±1%, use 80 dB.
For power line frequency ±3%, use 60 dB.
[5] Reading speeds for 60 Hz and (50 Hz) operation; autozero OFF
6 1/2 digits=22 bits, 5 1/2 digits=18 bits, 4 1/2 digits=15 bits
[7] Add 20 μV for DCV, 4 μA for DCI, or 20 mΩ for resistance
[8] For fixed function and range, readings to memory,
scaling and alarms off, autozero OFF

[1] 300 Vdc isolation voltage (ch-ch, ch-earth)

[2] For 1 kΩ unbalance in LO lead

[3] For power line frequency ±0.1%

[4] For power line frequency ±1%, use 80 dB.

For power line frequency ±3%, use 60 dB.

[5] Reading speeds for 60 Hz and (50 Hz) operation; autozero OFF

[6] 6 1/2 digits=22 bits, 5 1/2 digits=18 bits, 4 1/2 digits=15 bits

[7] Add 20 μV for DCV, 4 μA for DCI, or 20 mΩ for resistance

[8] For fixed function and range, readings to memory, scaling and alarms off, autozero OFF

Chapter 1 Specifications

AC Accuracy Specifications

■ AC Accuracy Specifications

± (% of reading + % of range)^[1]

Includes measurement error, switching error, and transducer conversion error

Includes measurement error, wiring error, and keyboard conversion error.							
Function	Range ^[3]	Frequency	24 Hour ^[2] 23 °C ± 1 °C	90 Day 23 °C ± 5 °C	1 Year 23 °C ± 5 °C	Temperature Coefficient /°C 0 °C – 18 °C 28 °C – 55 °C	
True RMS AC Voltage ^[4]	100.0000 mV to 100 V	3 Hz – 5 Hz	1.00 + 0.03	1.00 + 0.04	1.00 + 0.04	0.100 + 0.004	
		5 Hz – 10 Hz	0.35 + 0.03	0.35 + 0.04	0.35 + 0.04	0.035 + 0.004	
		10 Hz – 20 kHz	0.04 + 0.03	0.05 + 0.04	0.06 + 0.04	0.005 + 0.004	
		20 kHz – 50 kHz	0.10 + 0.05	0.11 + 0.05	0.12 + 0.05	0.011 + 0.005	
		50 kHz – 100 kHz	0.55 + 0.08	0.60 + 0.08	0.60 + 0.08	0.060 + 0.008	
		100 kHz – 300 kHz ^[5]	4.00 + 0.50	4.00 + 0.50	4.00 + 0.50	0.20 + 0.02	
	300.0000 V	3 Hz – 5 Hz	1.00 + 0.05	1.00 + 0.08	1.00 + 0.08	0.100 + 0.008	
		5 Hz – 10 Hz	0.35 + 0.05	0.35 + 0.08	0.35 + 0.08	0.035 + 0.008	
		10 Hz – 20 kHz	0.04 + 0.05	0.05 + 0.08	0.06 + 0.08	0.005 + 0.008	
		20 kHz – 50 kHz	0.10 + 0.10	0.11 + 0.12	0.12 + 0.12	0.011 + 0.012	
		50 kHz – 100 kHz	0.55 + 0.20	0.60 + 0.20	0.60 + 0.20	0.060 + 0.020	
		100 kHz – 300 kHz ^[5]	4.00 + 1.25	4.00 + 1.25	4.00 + 1.25	0.20 + 0.05	
Frequency and Period ^[6]	100 mV to 300 V	3 Hz – 5 Hz	0.10	0.10	0.10	0.005	
		5 Hz – 10 Hz	0.05	0.05	0.05	0.005	
		10 Hz – 40 Hz	0.03	0.03	0.03	0.001	
		40 Hz – 300 kHz	0.006	0.01	0.01	0.001	
True RMS AC Current <i>HP 34901A Only</i>	10.00000 mA ^[4] and 1.000000 A ^[4]	3 Hz – 5 Hz	1.00 + 0.04	1.00 + 0.04	1.00 + 0.04	0.100 + 0.006	
		5 Hz – 10 Hz	0.30 + 0.04	0.30 + 0.04	0.30 + 0.04	0.035 + 0.006	
		10 Hz – 5 kHz	0.10 + 0.04	0.10 + 0.04	0.10 + 0.04	0.015 + 0.006	
	100.0000 mA ^[7]	3 Hz – 5 Hz	1.00 + 0.5	1.00 + 0.5	1.00 + 0.5	0.100 + 0.06	
		5 Hz – 10 Hz	0.30 + 0.5	0.30 + 0.5	0.30 + 0.5	0.035 + 0.06	
		10 Hz – 5 kHz	0.10 + 0.5	0.10 + 0.5	0.10 + 0.5	0.015 + 0.06	
Additional Low Frequency Error for ACV, ACI (% of reading)				Additional Error for Frequency, Period (% of reading)			
Frequency	AC Filter Slow	AC Filter Medium	AC Filter Fast	Frequency	6½ Digits	5½ Digits	4½ Digits
10 Hz - 20 Hz	0	0.74	—	3 Hz - 5 Hz	0	0.12	0.12
20 Hz - 40 Hz	0	0.22	—	5 Hz - 10 Hz	0	0.17	0.17
40 Hz - 100 Hz	0	0.06	0.73	10 Hz - 40 Hz	0	0.2	0.2
100 Hz - 200 Hz	0	0.01	0.22	40 Hz - 100 Hz	0	0.06	0.21
200 Hz - 1 kHz	0	0	0.18	100 Hz - 300 Hz	0	0.03	0.21
> 1 kHz	0	0	0	300 Hz - 1 kHz	0	0.01	0.07
				> 1 kHz	0	0	0.02

[1] Specifications are for 1 hour warm up and 6½ digits, Slow ac filter

[2] Relative to calibration standards

[3] 20% over range on all ranges except 300 Vac and 1 Aac ranges

[4] For sinewave input > 5% of range. For inputs from 1% to 5% of range and < 50 kHz, add 0.1% of range additional error.

[5] Typically 30% of reading error at 1 MHz, limited to 1x10³ V Hz

[6] Input > 100 mV. For 10 mV inputs, multiply % of reading error x 10.

[7] Specified only for inputs > 10 mA

■ AC Measurement and Operating Characteristics

AC Measurement Characteristics ^[1]	
True RMS AC Voltage	
Measurement Method:	AC-coupled True RMS – measures the ac component of input with up to 300 Vdc of bias on any range
Crest Factor:	Maximum 5:1 at Full Scale
Additional Crest Factor Errors (non-sinewave): ^[2]	Crest Factor 1-2: 0.05% of reading Crest Factor 2-3: 0.15% of reading Crest Factor 3-4: 0.30% of reading Crest Factor 4-5: 0.40% of reading
AC Filter Bandwidth:	
Slow	3 Hz – 300 kHz
Medium	20 Hz – 300 kHz
Fast	200 Hz – 300 kHz
Input Impedance:	1 M Ω \pm 2%, in parallel with 150 pF
Input Protection:	300 Vrms on all ranges
Frequency and Period	
Measurement Method:	Reciprocal counting technique
Voltage Ranges:	Same as AC Voltage function
Gate Time:	1s, 100 ms, or 10 ms
Measurement Timeout:	Selectable 3 Hz, 20 Hz, 200 Hz LF limit
True RMS AC Current	
Measurement Method:	Direct coupled to the fuse and shunt. AC-coupled True RMS measurement (measures the ac component only)
Shunt Resistance:	5 Ω for 10 mA; 0.1 Ω for 100 mA, 1A
Input Protection:	1.5A 250 V fuse on HP 34901A module
Measurement Noise Rejection ^[3]	
AC CMRR:	70 dB
Measurement Considerations (Frequency and Period)	
All frequency counters are susceptible to error when measuring low-voltage, low-frequency signals. Shielding inputs from external noise pickup is critical for minimizing measurement errors.	

AC Operating Characteristics ^[4]			
Function	Digits ^[5]	Readings/s	AC Filter
ACV, ACI:	6½	7 sec/reading	Slow (3 Hz)
	6½	1	Medium (20 Hz)
	6½	8 ^[6]	Fast (200 Hz)
	6½	10	Fast (200 Hz)
	6½	100 ^[7]	Fast (200 Hz)
Single Channel Measurement Rates ^[8]			
Function	Resolution	Readings/s	
ACV:	6½ Slow (3 Hz)	0.14	
	6½ Medium (20 Hz)	1	
	6½ Fast (200 Hz)	8	
	6½ ^[7]	100	
Frequency, Period:	6½ Digits (1s gate)	0.77	
	6½ Digits (1s gate) ^[7]	1	
	5½ Digits (100 ms)	2.5	
	5½ Digits (100 ms) ^[7]	9	
	4½ Digits (10 ms)	3.2	
	4½ Digits (10 ms) ^[7]	70	

[1] 300 Vrms isolation voltage (ch-ch, ch-earth)

[2] For frequencies below 100 Hz, slow AC filter specified for sinewave input only

[3] For 1 k Ω unbalance in LO lead

[4] Maximum reading rates for 0.01% of ac step additional error. Additional settling delay required when input dc level varies.

[5] 6 1/2 digits=22 bits, 5 1/2 digits=18 bits, 4 1/2 digits=15 bits

[6] For external trigger or remote operation using default settling delay (Delay Auto)

[7] Maximum limit with default settling delays defeated

[8] For fixed function and range, readings to memory, scaling and alarms turned off

Chapter 1 Specifications
Measurement Rates and System Characteristics

■ Measurement Rates and System Characteristics

Single Channel Measurement Rates ^{[1] [2]}			System Characteristics	
Function	Resolution	Readings/s	Scan Triggering	
DCV, 2-Wire Ohms:	6½ (10 PLC)	6 (5)	Scan Count:	1 to 50,000 or continuous
	5½ (1 PLC)	57 (47)	Scan Interval:	0 to 99 hours; 1 ms step size
	4½ (0.02 PLC)	600	Channel Delay:	0 to 60 seconds/channel; 1 ms step size
Thermocouple:	0.1 °C (1 PLC) (0.02 PLC)	57 (47)	External Trig Delay:	< 5 ms; With Monitor On, < 200 ms
		220	External Trig Jitter:	< 2 ms
RTD, Thermistor:	0.01 °C (10 PLC)	6 (5)	Alarms	
	0.1 °C (1 PLC)	57 (47)	Alarm Outputs:	4 TTL compatible. Selectable TTL logic HI or LO on Fail
	1 °C (0.02 PLC)	220	Latency:	5 ms (typical)
ACV:	6½ Slow (3 Hz)	0.14	Memory	
	6½ Medium (20 Hz)	1	Readings:	Battery Backed, 4 year typical life ^[5] 50,000 readings
	6½ Fast (200 Hz)	8	States:	5 instrument states
	6½ ^[3]	100	Alarm Queue:	Up to 20 events
Frequency, Period:	6½ Digits (1s gate)	1	General Specifications	
	5½ Digits (100 ms)	9	Power Supply:	100 V / 120 V / 220 V / 240 V ±10%
	4½ Digits (10 ms)	70	Power Line Frequency:	45 Hz to 66 Hz automatically sensed
System Speeds ^[4]			Power Consumption:	(12 W) 25 VA peak
<i>INTO Memory</i>			Operating Environment:	Full accuracy for 0 °C to 55 °C Full accuracy to 80% R.H. at 40 °C
		Ch/s	Storage Environment:	-40 °C to 70 °C ^[5]
Single Channel DCV		600	Weight (Mainframe):	Net: 3.6 kg (8.0 lbs)
34902A Scanning DCV		250	Safety:	Conforms to CSA, UL-1244, IEC 1010 Cat I
34907A Scanning Digital Input		250	RFI and ESD:	CISPR 11, IEC 801/2/3/4
34902A Scanning DCV, scaling and 1 alarm fail		220	Warranty:	3 years
34907A Scanning Totalize		170	^[1] Reading speeds for 60 Hz and (50 Hz) operation; autozero OFF ^[2] For fixed function and range, readings to memory, scaling and alarms off, autozero OFF ^[3] Maximum limit with default settling delays defeated ^[4] Speeds are for 4½ digits, delay 0, display off, autozero off. Using 115 kbaud RS-232 setting. ^[5] Storage at temperatures above 40 °C will decrease battery life	
34902A Scanning Temperature		160		
34902A Scanning ACV ^[3]		100		
34902A Scanning DCV/Ohms, alternate channels		90		
34901A/34908A Scanning DCV		60		
<i>INTO and OUT of Memory to HP-IB or RS-232 (INIT, FETCh)</i>				
34902A Scanning DCV		180		
34902A Scanning DCV with Time stamp		150		
<i>OUT of Memory to HP-IB</i>				
Readings		800		
Readings with Time stamp		450		
Readings with all Format Options ON		310		
<i>OUT of Memory to RS-232</i>				
Readings		600		
Readings with Time stamp		320		
Readings with all Format Options ON		230		
<i>DIRECT to HP-IB or RS-232</i>				
Single Channel DCV		440		
34902A Scanning DCV		200		
Single Channel MEAS DCV 10 or MEAS DCV 1		25		
Single Channel MEAS DCV or MEAS OHMS		12		

■ Module Specifications

HP 34901A, 34902A, 34908A, 34903A, 34904A

	Multiplexer			Actuator	Matrix
General	34901A	34902A	34908A	34903A	34904A
Number of Channels	20+2	16	40	20	4x8
	2/4 wire	2/4 wire	1 wire	SPDT	2 wire
Connects to Internal DMM	Yes	Yes	Yes	No	No
Scanning Speed	60 ch/s	250 ch/s	60 ch/s		
Open/Close Speed	120/s	120/s	70/s	120/s	120/s
Maximum Input					
Voltage (dc, ac rms)	300 V	300 V	300 V	300 V	300 V
Current (dc, ac rms)	1 A	50 mA	1 A	1 A	1 A
Power (W, VA)	50 W	2 W	50 W	50 W	50 W
Isolation (ch-ch, ch-earth) dc, ac rms	300 V	300 V	300 V	300 V	300 V
DC Characteristics					
Offset Voltage ^[1]	< 3 μ V	< 6 μ V	< 3 μ V	< 3 μ V	< 3 μ V
Initial Closed Channel R ^[1]	< 1 Ω	< 1 Ω	< 1 Ω	< 0.2 Ω	< 1 Ω
Isolation (ch-ch, ch-earth)	> 10 G Ω	> 10 G Ω	> 10 G Ω	> 10 G Ω	> 10 G Ω
AC Characteristics					
Bandwidth	10 MHz	10 MHz	10 MHz	10 MHz	10 MHz
Ch-Ch Cross Talk (dB) ^[2] 10 MHz	-45	-45	-18 ^[3]	-45	-33
Capacitance HI to LO	< 50 pF	< 50 pF	< 50 pF	< 10 pF	< 50 pF
Capacitance LO to Earth	< 80 pF	< 80 pF	< 80 pF	< 80 pF	< 80 pF
Volt-Hertz Limit	10 ⁸	10 ⁸	10 ⁸	10 ⁸	10 ⁸
Other					
T/C Cold Junction Accuracy ^[1] (typical)	0.8 °C	0.8 °C	0.8 °C		
Switch Life No Load (typical)	100M	100M	100M	100M	100M
Switch Life Rated Load (typical) ^[4]	100k	100k	100k	100k	100k
Temperature Operating	All Modules - 0 °C to 55 °C				
Temperature Storage	All Modules - -20 °C to 70 °C				
Humidity (non-condensing)	All Modules - 40 °C / 80% R.H.				

[1] Errors included in the DMM measurement accuracy specifications

[2] 50 Ω source, 50 Ω load

[3] Isolation within channel 1 to 20 or 21 to 40 banks is -40 dB

[4] Applies to resistive loads only

Chapter 1 Specifications

Module Specifications

■ Module Specifications

HP 34905A, 34906A

	RF Multiplexer	
General	34905A	34906A
Number of Channels	Dual 1x4 50Ω	Dual 1x4 75Ω
Open/Close Speed	60/s	
Maximum Input		
Voltage (dc, ac rms)	42 V	
Current (dc, ac rms)	0.7 A	
Power (W, VA)	20 W	
DC Characteristics		
Offset Voltage ^[1]	< 6 μV	
Initial Closed Channel R ^[1]	< 0.5Ω	
Isolation (ch-ch, ch-earth)	> 1 GΩ	
Other		
Switch Life No Load (typical)	5M	
Switch Life Rated Load (typical) ^[2]	100k	
Temperature Operating	0 °C to 55 °C	
Temperature Storage	-20 °C to 70 °C	
Humidity (non-condensing)	40 °C / 80% R.H.	

The ac performance graphs are shown on the following page.

AC Characteristics		34905A	34906A
Bandwidth ^[3]		2 GHz	2 GHz
Insertion Loss (dB)	10 MHz	-0.1	-0.1
	100 MHz	-0.4	-0.4
	500 MHz	-0.6	-0.5
	1 GHz	-1.0	-1.0
	1.5 GHz	-1.2	-1.5
SWR	2 GHz	-3.0	-2.0
	10 MHz	1.02	1.02
	100 MHz	1.05	1.05
	500 MHz	1.20	1.25
	1 GHz	1.20	1.40
Ch-Ch Cross Talk (dB) ^[4]	1.5 GHz	1.30	1.40
	2 GHz	1.40	2.00
	10 MHz	-100	-85
	100 MHz	-85	-75
	500 MHz	-65	-65
Risetime	1 GHz	-55	-50
	1.5 GHz	-45	-40
	2 GHz	-35	-35
Signal Delay		< 300 ps	
Capacitance	HI to LO	< 20 pF	
Volt-Hertz Limit		10 ¹⁰	

[1] Errors included in DMM measurement accuracy specifications

[2] Applies to resistive loads only


[3] Bandwidth direct to module SMB connectors

[4] 50Ω source, 50Ω load


■ Typical AC Performance Graphs

HP 34905A, 34906A

Insertion Loss (50Ω)

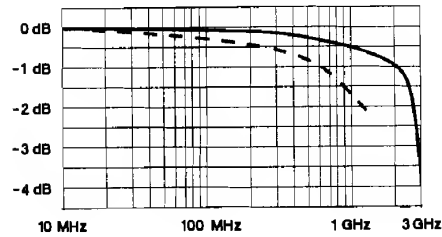


Insertion Loss (75Ω)

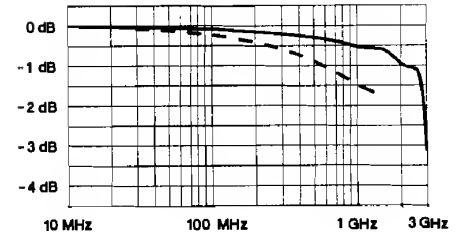


— Direct to Module
- - - Using provided adapter cables


VSWR (50Ω)

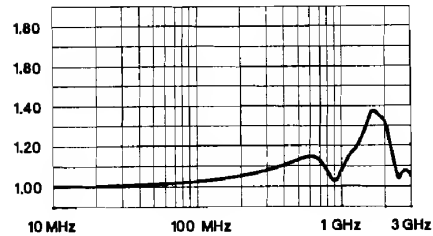


VSWR (75Ω)

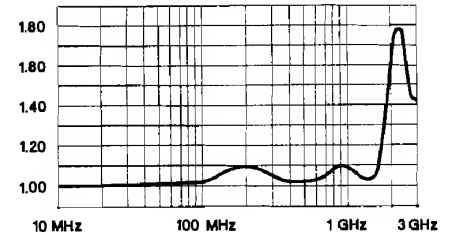

Crosstalk (50Ω)

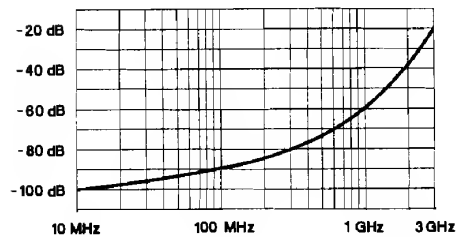

Crosstalk (75Ω)

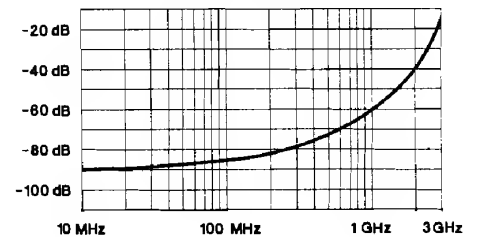

Chapter 1 Specifications

Module Specifications

■ Module Specifications

HP 34907A

Digital Input/Output

Port 1, 2:	8 Bit, input or output, non-isolated
Vin(L):	< 0.8V (TTL)
Vin(H):	> 2.0V (TTL)
Vout(L):	< 0.8V @ Iout = -400 mA
Vout(H):	> 2.4V @ Iout = 1 mA
Vout(H) Max:	< 42V with external open drain pull-up
Alarming:	Maskable pattern match or state change
Speed	4 ms (max) alarm sampling
Latency	5 ms (typical) to 34970A alarm output
Read/Write Speed:	95/s

Totalize Input

Maximum Count:	2 ²⁶ - 1 (67,108,863)
Totalize Input:	100 kHz (max), rising or falling edge, programmable
Signal Level:	1 Vp-p (min) 42 Vpk (max)
Threshold:	0V or TTL, jumper selectable
Gate Input:	TTL-Hi, TTL-Lo, or none
Count Reset:	Manual or Read+Reset
Read Speed:	85/s

Analog Voltage (DAC) Output

DAC 1, 2:	±12V, non-isolated
Resolution:	1 mV
Iout:	10 mA max
Settling Time:	1 ms to 0.01% of output
Accuracy:	±(% of output + mV)
1 year ±5 °C	0.15% + 6 mV
90 day ±5 °C	0.1% + 6 mV
24 hour ±1 °C	0.04% + 4 mV
Temp Coefficient:	±(0.015% + 1 mV) / °C

■ Software Specifications

HP BenchLink Data Logger *(not included with Option 001)*

System Requirements ^[1]

PC Hardware:	486, 66 MHz, 16 MB RAM, 12 MB disk space
Operating System:	Windows® 3.1, Windows 95, Windows NT® 4.0

Computer Interfaces ^[2]

HP-IB:	HP 82335B, 82340A/B/C, 82341A/B/C/D National Instruments AT-GPIB/TNT, PCI-GPIB
LAN-to-HP-IB:	HP E2050A (Windows 95 and NT only)
RS-232 (Serial Port):	PC COM 1 to 4

Performance ^[3]



Scan and Save to Disk:	100 ch/s, 2 strip charts displayed
------------------------	------------------------------------

[1] Software provided on CD-ROM; includes utility to create floppy disks for installation

[2] Interface and drivers must be purchased and installed separately

[3] 90 MHz Pentium®, 20 MB RAM

■ Product and Module Dimensions

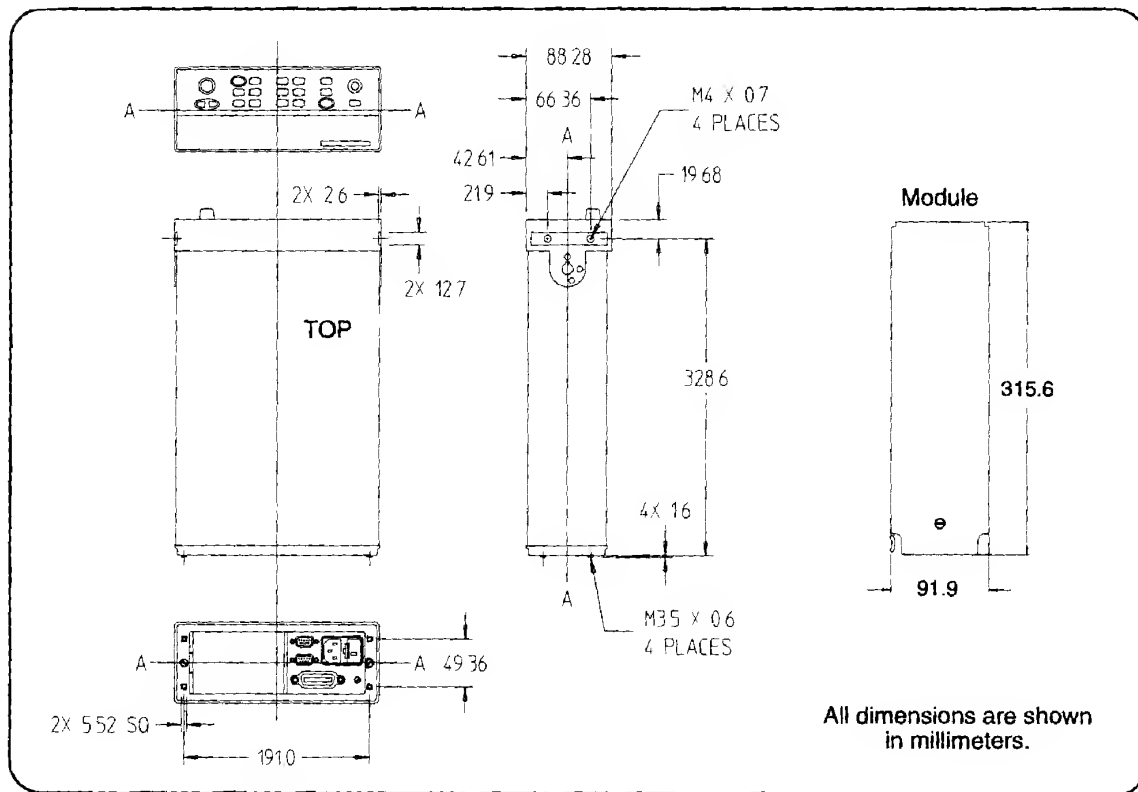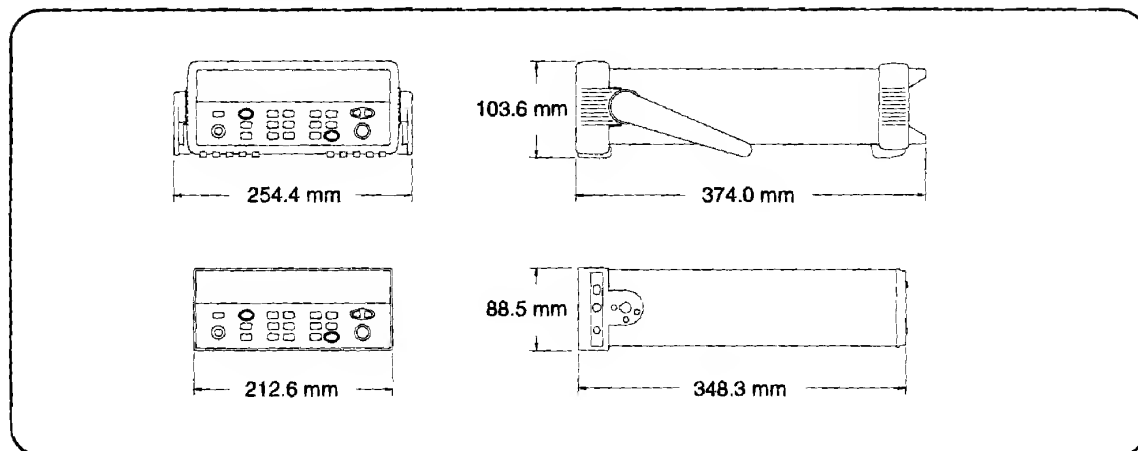

To Calculate Total Measurement Error

Each specification includes correction factors which account for errors present due to operational limitations of the internal DMM. This section explains these errors and shows how to apply them to your measurements. Refer to “Interpreting Internal DMM Specifications,” starting on page 28, to get a better understanding of the terminology used and to help you interpret the internal DMM’s specifications.

The internal DMM’s accuracy specifications are expressed in the form: (*% of reading + % of range*). In addition to the reading error and range error, you may need to add additional errors for certain operating conditions. Check the list below to make sure you include all measurement errors for a given function. Also, make sure you apply the conditions as described in the footnotes on the specification pages.

- If you are operating the internal DMM outside the $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ temperature range specified, apply an additional *temperature coefficient error*.
- For dc voltage, dc current, and resistance measurements, you may need to apply an additional *reading speed error*.
- For ac voltage and ac current measurements, you may need to apply an additional *low frequency error* or *crest factor error*.

Understanding the “% of reading” Error The *reading error* compensates for inaccuracies that result from the function and range you select, as well as the input signal level. The reading error varies according to the input level on the selected range. This error is expressed in percent of reading. The following table shows the reading error applied to the internal DMM’s 24-hour dc voltage specification.

Range	Input Level	Reading Error (% of reading)	Reading Error Voltage
10 Vdc	10 Vdc	0.0015	$\leq 150\text{ }\mu\text{V}$
10 Vdc	1 Vdc	0.0015	$\leq 15\text{ }\mu\text{V}$
10 Vdc	0.1 Vdc	0.0015	$\leq 1.5\text{ }\mu\text{V}$

Understanding the “% of range” Error The *range error* compensates for inaccuracies that result from the function and range you select. The range error contributes a constant error, expressed as a percent of range, *independent* of the input signal level. The following table shows the range error applied to the DMM’s 24-hour dc voltage specification.

Range	Input Level	Range Error (% of range)	Range Error Voltage
10 Vdc	10 Vdc	0.0004	≤ 40 μV
10 Vdc	1 Vdc	0.0004	≤ 40 μV
10 Vdc	0.1 Vdc	0.0004	≤ 40 μV

Total Measurement Error To compute the total measurement error, add the reading error and range error. You can then convert the total measurement error to a “percent of input” error or a “ppm (part-per-million) of input” error as shown below.

$$\% \text{ of input error} = \frac{\text{Total Measurement Error}}{\text{Input Signal Level}} \times 100$$

$$\text{ppm of input error} = \frac{\text{Total Measurement Error}}{\text{Input Signal Level}} \times 1,000,000$$

Example: Computing Total Measurement Error

Assume that a 5 Vdc signal is input to the DMM on the 10 Vdc range. Compute the total measurement error using the 90-day accuracy specification of ±(0.0020% of reading + 0.0005% of range).

$$\text{Reading Error} = 0.0020\% \times 5 \text{ Vdc} = 100 \mu\text{V}$$

$$\text{Range Error} = 0.0005\% \times 10 \text{ Vdc} = 50 \mu\text{V}$$

$$\begin{aligned} \text{Total Error} &= 100 \mu\text{V} + 50 \mu\text{V} = \pm 150 \mu\text{V} \\ &= \pm 0.0030\% \text{ of } 5 \text{ Vdc} \\ &= \pm 30 \text{ ppm of } 5 \text{ Vdc} \end{aligned}$$

Interpreting Internal DMM Specifications

This section is provided to give you a better understanding of the terminology used and will help you interpret the internal DMM's specifications.

Number of Digits and Overrange

The “number of digits” specification is the most fundamental, and sometimes, the most confusing characteristic of a multimeter. The number of digits is equal to the maximum number of “9’s” the multimeter can measure or display. This indicates the number of *full digits*. Most multimeters have the ability to overrange and add a partial or “½” digit.

For example, the internal DMM can measure 9.99999 Vdc on the 10 V range. This represents six full digits of resolution. The internal DMM can also overrange on the 10 V range and measure up to a maximum of 12.00000 Vdc. This corresponds to a 6½-digit measurement with 20% overrange capability.

Sensitivity

Sensitivity is the minimum level that the multimeter can detect for a given measurement. Sensitivity defines the ability of the multimeter to respond to small changes in the input level. For example, suppose you are monitoring a 1 mVdc signal and you want to adjust the level to within $\pm 1 \mu\text{V}$. To be able to respond to an adjustment this small, this measurement would require a multimeter with a sensitivity of at least $1 \mu\text{V}$. You could use a 6½-digit multimeter *if* it has a 1 Vdc or smaller range. You could also use a 4½-digit multimeter with a 10 mVdc range.

For ac voltage and ac current measurements, note that the smallest value that can be measured is different from the sensitivity. For the internal DMM, these functions are specified to measure down to 1% of the selected range. For example, the internal DMM can measure down to 1 mV on the 100 mV range.

Resolution

Resolution is the numeric ratio of the maximum displayed value divided by the minimum displayed value on a selected range. Resolution is often expressed in percent, parts-per-million (ppm), counts, or bits. For example, a 6½-digit multimeter with 20% overrange capability can display a measurement with up to 1,200,000 counts of resolution. This corresponds to about 0.0001% (1 ppm) of full scale, or 21 bits including the sign bit. All four specifications are equivalent.

Accuracy

Accuracy is a measure of the “exactness” to which the internal DMM’s measurement uncertainty can be determined *relative* to the calibration reference used. Absolute accuracy includes the Internal DMM’s relative accuracy specification plus the known error of the calibration reference relative to national standards (such as the U.S. National Institute of Standards and Technology). To be meaningful, the accuracy specifications must be accompanied with the conditions under which they are valid. These conditions should include temperature, humidity, and time.

There is no standard convention among multimeter manufacturers for the confidence limits at which specifications are set. The table below shows the probability of non-conformance for *each specification* with the given assumptions.

Specification Criteria	Probability of Failure
Mean \pm 2 sigma	4.5%
Mean \pm 3 sigma	0.3%

Variations in performance from reading to reading, and instrument to instrument, decrease for increasing number of sigma for a given specification. This means that you can achieve greater actual measurement precision for a specific accuracy specification number. The HP 34970A is designed and tested to meet performance better than mean \pm 3 sigma of the published accuracy specifications.

24-Hour Accuracy

The 24-hour accuracy specification indicates the internal DMM's relative accuracy over its full measurement range for short time intervals and within a stable environment. Short-term accuracy is usually specified for a 24-hour period and for a $\pm 1\text{ }^{\circ}\text{C}$ temperature range.

90-Day and 1-Year Accuracy

These long-term accuracy specifications are valid for a $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ temperature range. These specifications include the initial calibration errors plus the internal DMM's long-term drift errors.

Temperature Coefficients

Accuracy is usually specified for a $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ temperature range. This is a common temperature range for many operating environments. You must add additional temperature coefficient errors to the accuracy specification if you are operating the multimeter outside a $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ temperature range (the specification is per $^{\circ}\text{C}$).

Configuring for Highest Accuracy Measurements

The measurement configurations shown below assume that the internal DMM is in its *Factory Reset* state. It is also assumed that manual ranging is enabled to ensure proper full scale range selection.

DC Voltage, DC Current, and Resistance Measurements:

- Set the resolution to 6 digits (you can use the 6 digits slow mode for further noise reduction).
- Set the input resistance to greater than 10 G Ω (for the 100 mV, 1 V, and 10 V ranges) for the best dc voltage accuracy.
- Use 4-wire ohms and enable offset compensation for the best resistance accuracy.

AC Voltage and AC Current Measurements:

- Set the resolution to 6 digits.
- Select the slow ac filter (3 Hz to 300 kHz).




Frequency and Period Measurements:


- Set the resolution to 6 digits.

Quick Start

Quick Start

One of the first things you will want to do with your instrument is to become acquainted with the front panel. We have written the exercises in this chapter to prepare the instrument for use and help you get familiar with some of its front-panel operations.

The front panel has several groups of keys to select various functions and operations. A few keys have a *shifted* function printed in blue below the key. To perform a shifted function, press  (the **SHIFT** annunciator will turn on). Then, press the key that has the desired label below it. For example, to select the Utility Menu, press  .

If you accidentally press , just press it again to turn off the **SHIFT** annunciator.

This chapter is divided into the following sections:

- To Prepare the Instrument for Use, *on page 35*
- To Connect Wiring to a Module, *on page 36*
- To Set the Time and Date, *on page 38*
- To Configure a Measurement Channel, *on page 39*
- To Monitor a Single Channel, *on page 40*
- To Close a Channel, *on page 41*
- If the Instrument Does Not Turn On, *on page 42*
- To Adjust the Carrying Handle, *on page 44*
- To Rack Mount the Instrument, *on page 45*

To Prepare the Instrument for Use

1 Check the list of supplied items.

Verify that you have received the following items with your instrument. If anything is missing, contact your nearest Hewlett-Packard Sales Office.

- ☐ One power cord.
- ☐ One *User's Guide*.
- ☐ This *Service Guide*.
- ☐ One *Quick Reference Guide*.
- ☐ Certificate of Calibration (if you ordered the internal DMM).
- ☐ Quick Start Kit (if you ordered the internal DMM):
 - One RS-232 cable.
 - HP BenchLink Data Logger Software CD-ROM.
 - One J-type thermocouple and a flatblade screwdriver.
- ☐ Any plug-in modules that you ordered are delivered in a separate shipping container.




On/Standby
Switch


WARNING

*Note that this switch is **Standby** only. To disconnect the mains from the instrument, remove the power cord.*

2 Connect the power cord and turn on the instrument.


The front-panel display will light up briefly while the instrument performs its power-on self-test. The HP-IB address is displayed. The instrument initially powers up with all measurement channels turned off. To review the power-on display with all annunciators turned on, hold down  as you turn on the instrument. *If the instrument does not turn on properly, see page 42.*

3 Perform a complete self-test.


The *complete* self-test performs a more extensive set of tests than those performed at power-on. Hold down  as you turn on the instrument and *hold down the key until you hear a long beep*. The self-test will begin when you release the key following the beep.

To Connect Wiring to a Module


1 Remove the module cover.

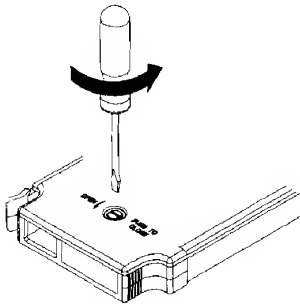


2 Connect wiring to the screw terminals.

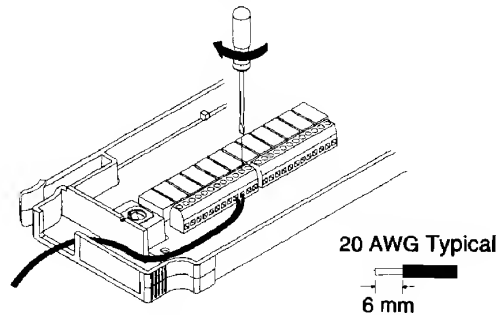


3 Route wiring through strain relief.

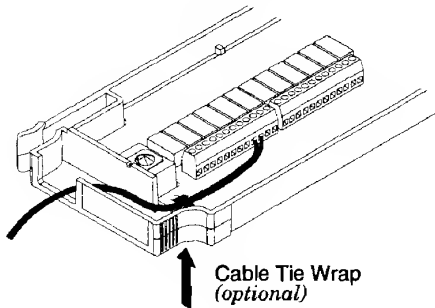

4 Replace the module cover.

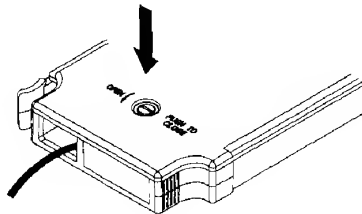


5 Install the module into mainframe.

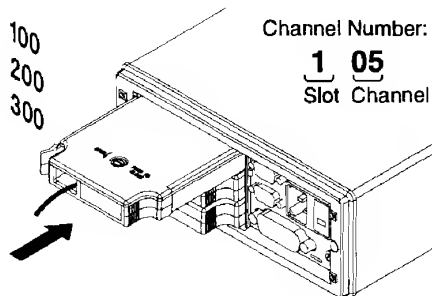

Wiring Hints...


- For detailed information on each module, refer to the *HP 34970A User's Guide*.
- To reduce wear on the internal DMM relays, wire *like* functions on adjacent channels.
- Use shielded twisted pair Teflon® insulated cables to reduce settling and noise errors.
- The diagrams on the next page show how to connect wiring to a multiplexer module for each measurement function. ➔

Thermocouple

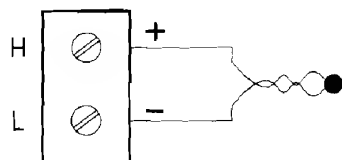


Thermocouple Types: B, E, J, K, N, R, S, T

DC Voltage / AC Voltage / Frequency




Ranges: 100 mV, 1 V, 10 V, 100 V, 300 V

2-Wire Ohms / RTD / Thermistor



Ranges: 100, 1 k, 10 k, 100 k, 1 M, 10 M, 100 M Ω
RTD Types: 0.00385, 0.00391
Thermistor Types: 2.2 k, 5 k, 10 k


4-Wire Ohms / RTD

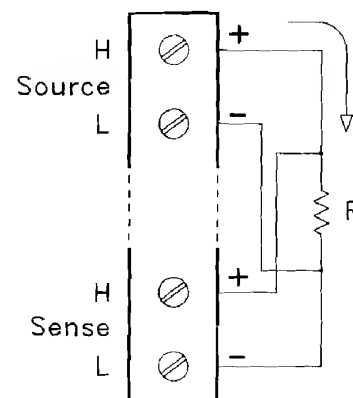

Channel n (source) is automatically paired with
Channel $n+10$ (sense) on the HP 34901A or
Channel $n+8$ (sense) on the HP 34902A.

Ranges: 100, 1 k, 10 k, 100 k, 1 M, 10 M, 100 M Ω
RTD Types: 0.00385, 0.00391


DC Current / AC Current

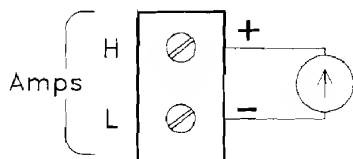

Valid only on channels 21 and 22 on the HP 34901A.
Ranges: 10 mA, 100 mA, 1A

To Set the Time and Date

All readings during a scan are automatically time stamped and stored in non-volatile memory. In addition, alarm data is time stamped and stored in a separate non-volatile memory queue.



1 Set the time of day.

Use ◀ and ▶ to select the field to modify and turn the knob to change the value. You can also edit the AM/PM field.

TIME 03:45 PM



2 Set the date.

Use ◀ and ▶ to select the field to modify and turn the knob to change the value.

MAY 01 1997

To Configure a Measurement Channel

Use this general procedure to configure a measurement channel.




1 Select the channel.

Turn the knob until the desired channel is shown on the right side of front-panel display. The channel number is a three-digit number; the left-most digit represents the slot number (100, 200, or 300) and the two digits on the right indicate the channel number (102, 110, etc.).

Note: You can use ◀ and ▶ to skip to the beginning of the previous or next slot.



2 Select the measurement parameters for the selected channel.

Use the knob to scroll through the measurement choices on each level of the menu. When you press  to make your selection, the menu automatically guides you through all relevant choices to configure a measurement on the selected function. When you have finished configuring the parameters, you are automatically exited from the menu.

The present selection (or default) is displayed in full bright for easy identification. When you make a different selection, the new choice is shown in full bright and it becomes the default selection. The order of the choices always remains the same; however, you always enter the menu at the present (full-bright) setting for each parameter.

Note: The menu will timeout after about 20 seconds of inactivity and any changes made previously will take effect.

To Monitor a Single Channel

You can use the *Monitor* function to continuously take readings on a single channel, even during a scan. This feature is used during front panel calibration procedures.




1 Select the channel to be monitored.

Only one channel can be monitored at a time but you can change the channel being monitored at any time by turning the knob.



2 Enable monitoring on the selected channel.

Any channel that can be “read” by the instrument can be monitored (the **MON** annunciator turns on). This includes any combination of temperature, voltage, resistance, current, frequency, or period measurements on multiplexer channels. You can also monitor a digital input port or the totalizer count on the multifunction module.

To disable monitoring, press  again.

To Close a Channel

On the multiplexer and switch modules, you can close and open individual relays on the module. However, note that if you have already configured any multiplexer channels for scanning, you cannot independently close and open individual relays on that module.



1 Select the channel.


Turn the knob until the desired channel is shown on the right side of front-panel display. For this example, select channel 213.









2 Close the selected channel.



3 Open the selected channel.

Note:  will sequentially open all channels on the module in the selected slot.

The table below shows the low-level control operations available for each of the plug-in modules.

Plug-In Module					 , 
34901A 20-Channel Mux	•	•	•		•
34902A 16-Channel Mux	•	•	•		•
34908A 40-Channel Single-Ended Mux ^[1]	•	•	•		•
34903A 20-Channel Actuator	•	•			
34904A 4x8 Matrix	•	•			
34905A Dual 4-Channel RF Mux (50Ω) ^[2]	•				
34906A Dual 4-Channel RF Mux (75Ω) ^[2]	•				
34907A Multifunction Module (DIO)			•	•	•
34907A Multifunction Module (Totalizer)			•		•
34907A Multifunction Module (DAC)				•	

[1] Only one channel can be closed at a time on this module.


[2] Only one channel in each bank can be closed at a time on this module.

If the Instrument Does Not Turn On

Use the following steps to help solve problems you might encounter when turning on the instrument.

1 Verify that there is ac power to the instrument.

First, verify that the power cord is firmly plugged into the power receptacle on the rear panel of the instrument. You should also make sure that the power source you plugged the instrument into is energized. Then, verify that the instrument is turned on.

The On/Standby switch  is located on the lower left side of the front panel.

2 Verify the power-line voltage setting.

The line voltage is set to the proper value for your country when the instrument is shipped from the factory. Change the voltage setting if it is not correct. The settings are: 100, 120, 220, or 240 Vac.

Note: For 127 Vac operation, use the 120 Vac setting.
For 230 Vac operation, use the 220 Vac setting.

See the next page if you need to change the line-voltage setting.

3 Verify that the power-line fuse is good.


The instrument is shipped from the factory with a 500 mA fuse installed. This is the correct fuse for all line voltages.

See the next page if you need to replace the power-line fuse.


To replace the 500 mA, 250 V fuse, order HP part number 2110-0458.

Chapter 2 Quick Start
If the Instrument Does Not Turn On

- 1 Remove the power cord.** Remove the fuse-holder assembly from the rear panel.

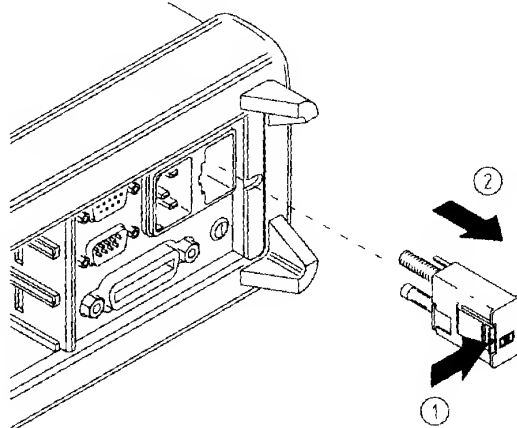


- 2 Remove the line-voltage selector** from the assembly.

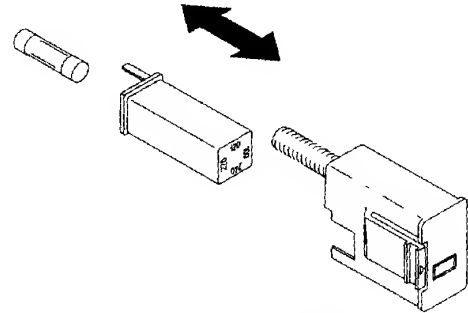


Fuse: 500 mA (for all line voltages)
Part Number: 2110-0458

- 3 Rotate the line-voltage selector** until the correct voltage appears in the window.

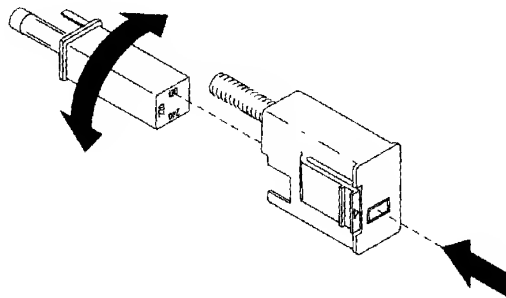

100, 120 (127), 220 (230) or 240 Vac

- 4 Replace the fuse-holder assembly** in the rear panel.


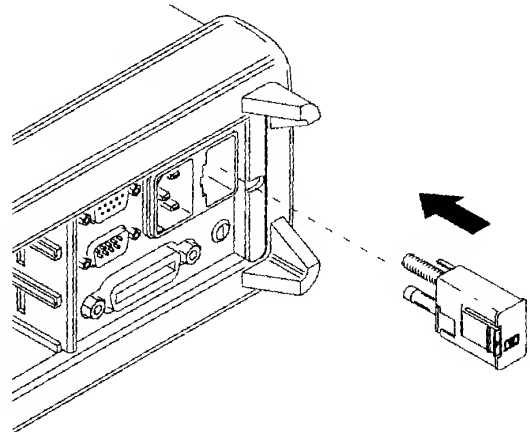


Verify that the correct line voltage is selected and the power-line fuse is good.


To Adjust the Carrying Handle

To Adjust the Carrying Handle

To adjust the position, grasp the handle by the sides and *pull outward*. Then, rotate the handle to the desired position.

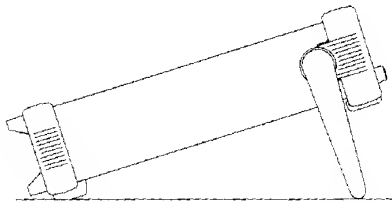

Benchtop Viewing Positions




Carrying Position


To Rack Mount the Instrument

You can mount the instrument in a standard 19-inch rack cabinet using one of three optional kits available. Instructions and mounting hardware are included with each rack-mounting kit. Any HP *System II* instrument of the same size can be rack-mounted beside the HP 34970A.

Remove the carrying handle, and the front and rear rubber bumpers, before rack-mounting the instrument.

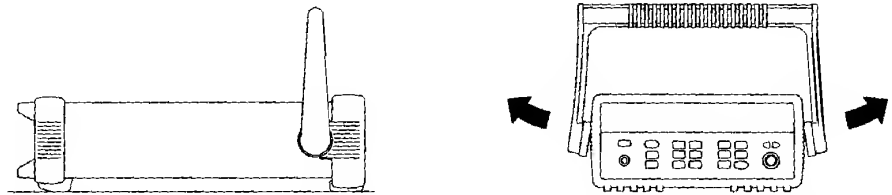


To remove the handle, rotate it to the vertical position and pull the ends outward.

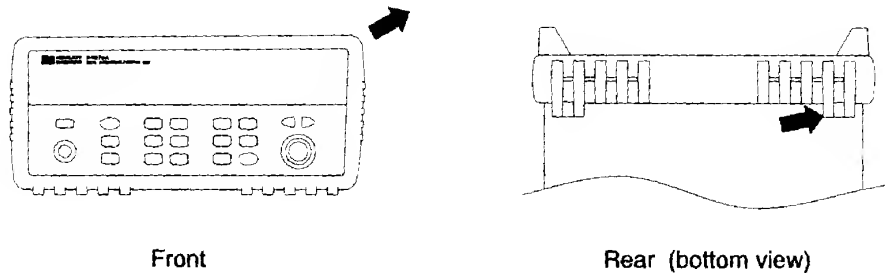


To remove the rubber bumper, stretch a corner and then slide it off.


Chapter 2 Quick Start
To Rack Mount the Instrument

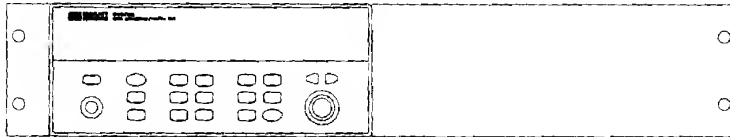

To rack mount a single Instrument, order adapter kit 5063-9240.

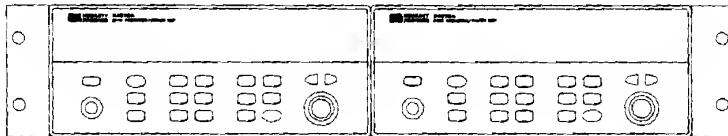

To rack mount two instruments side-by-side, order lock-link kit 5061-9694 and flange kit 5063-9212. Be sure to use the support rails inside the rack cabinet.

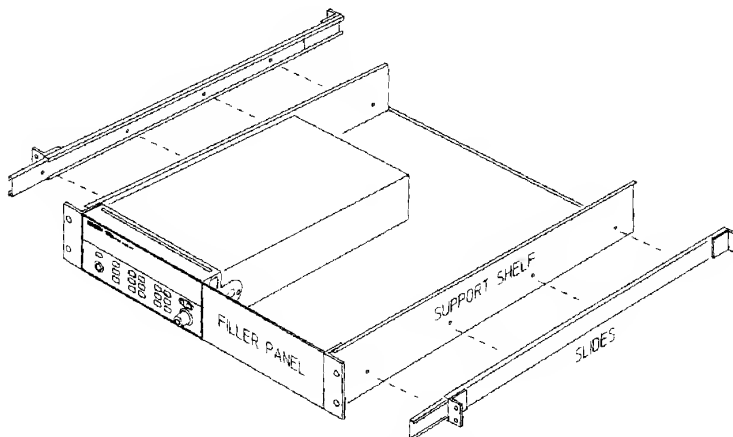

To install one or two instruments in a sliding support shelf, order shelf 5063-9255, and slide kit 1494-0015 (for a single instrument, also order filler panel 5002-3999).

Front-Panel Overview

Front-Panel Overview

This chapter introduces you to the front-panel keys and menu operation. This chapter does not give a detailed description of every front-panel key or menu operation. It does, however, give you a good overview of the front-panel menu and many front-panel operations. See the *HP 34970A User's Guide* for a complete discussion of the instrument's capabilities and operation.

This chapter is divided into the following sections:

- Front-Panel Menu Reference, *on page 49*
- To Unsecure for Calibration, *on page 51*
- To Secure Against Calibration, *on page 51*
- To Change the Security Code, *on page 52*
- Error Message, *on page 52*
- To Perform a Zero Adjustment, *on page 81*
- To Apply $Mx+B$ Scaling to Measurements, *on page 54*
- To Read the Relay Cycle Count, *on page 55*
- To Read a Digital Input Port, *on page 56*
- To Write to a Digital Output Port, *on page 57*
- To Read the Totalizer Count, *on page 58*
- To Output a DC Voltage, *on page 59*

Front-Panel Menu Reference

This section gives an overview of the front-panel menus. The menus are designed to automatically guide you through all parameters required to configure a particular function or operation. The remainder of this chapter shows examples of using the front-panel menus.



Configure the measurement parameters on the displayed channel.

- Select measurement function (dc volts, ohms, etc.) on the displayed channel.
- Select transducer type for temperature measurements.
- Select units (°C, °F, or K) for temperature measurements.
- Select measurement range or autorange.
- Select measurement resolution.
- Copy and paste measurement configuration to other channels.



Configure the scaling parameters for the displayed channel.

- Set the gain ("M") and offset ("B") value for the displayed channel.
- Make a null measurement and store it as the offset value.
- Specify a custom label (RPM, PSI, etc.) for the displayed channel.



Configure alarms on the displayed channel.

- Select one of four alarms to report alarm conditions on the displayed channel.
- Configure a high limit, low limit, or both for the displayed channel.
- Configure a bit pattern which will generate an alarm (for digital input channels).



Configure the four Alarm Output hardware lines.

- Clear the state of the four alarm output lines.
- Select the "Latch" or "Track" mode for the four alarm output lines.
- Select the slope (rising or falling edge) for the four alarm output lines.



Configure the event or action that controls the scan interval.

- Select the scan interval mode (interval, manual, external, or alarm).
- Select the scan count.

Chapter 3 Front-Panel Overview

Front-Panel Menu Reference

Advanced

Configure the advanced measurement features on displayed channel.

- Set the integration time for measurements on the displayed channel.
- Set the channel-to-channel delay for scanning.
- Enable/disable the thermocouple check feature (T/C measurements only).
- Select the reference junction source (T/C measurements only).
- Set the low frequency limit (ac measurements only).
- Enable/disable offset compensation (resistance measurements only).
- Select the binary or decimal mode for digital operations (HP 34907A only).
- Configure the totalizer reset mode (totalizer only).
- Select which edge is detected (rising or falling) for totalizer operations.

Utility

Configure system-related instrument parameters.

- Set the real-time system clock and calendar.
- Query the firmware revisions for the mainframe and installed modules.
- Select the instrument's power-on configuration (last or factory reset).
- Enable/disable the internal DMM.
- Secure/unsecure the instrument for calibration.

View

View readings, alarms, and errors.

- View the last 100 scanned readings from memory (last, min, max, and average).
- View the first 20 alarms in the alarm queue (reading and time alarm occurred).
- View up to 10 errors in the error queue.
- Read the number of cycles for the displayed relay (relay maintenance feature).

Sto/Rec

Store and recall instrument states.

- Store up to five instrument states in non-volatile memory.
- Assign a name to each storage location.
- Recall stored states, power-down state, factory reset state, or preset state.


Interface



Configure the remote interface.

- Select the HP-IB address.
- Configure the RS-232 interface (baud rate, parity, and flow control).

To Unsecure for Calibration

You can unsecure the instrument either from the front panel or over the remote interface. The instrument is secured when shipped from the factory and the security code is set to “HP034970”.


- Once you enter a security code, that code must be used for both front-panel and remote operation. For example if you secure the instrument from the front panel, you must use that same code to unsecure it from the remote interface.
- Press  to enter the *Utility* menu.



When you first enter the *Utility* menu, the calibration entries toggle between CAL SECURED and UNSECURE CAL. To unsecure the instrument, select UNSECURE CAL and press . After entering the correct security code, press  again. When you return to the menu, you will see new choices CAL UNSECURED and SECURE CAL.

Note: If you enter the wrong secure code, NO MATCH is displayed and a new choice, EXIT, is shown.


To Secure Against Calibration

You can secure the instrument either from the front panel or over the remote interface. The instrument is secured when shipped from the factory and the security code is set to “HP034970”.

- Once you enter a security code, that code must be used for both front-panel and remote operation. For example if you secure the instrument from the front panel, you must use that same code to unsecure it from the remote interface.
- Press  to enter the *Utility* menu.


When you enter the *Utility* menu, the calibration entries toggle between CAL UNSECURED and SECURE CAL. To secure the instrument, select SECURE CAL and press . After entering the desired security code, press  again. When you return to the menu, you will see new choices CAL SECURED and UNSECURE CAL.

To Change the Security Code

- To change the security code, you must first unsecure the instrument, and then enter a new code. Make sure you have read the security code rules described on page 67 before attempting to change the security code.
- To change the security code, first make sure that the instrument is unsecured. Go to the SECURE CAL entry, enter the new security code, and press  (the instrument is now secured with the new code). Changing the code from the front panel also changes the code as seen from the remote interface.

Error Messages

Error messages are retrieved in a first-in first-out (FIFO) order.

When the ERROR annunciator is on, press  to view error messages. Use the arrow keys to scroll the message in the display.

A list of the self-test errors messages and their meanings begin on page 150.

For a complete list of error messages and descriptions, see chapter 6 in the *HP 34970A User's Guide*.

To Perform a Zero Adjustment

The instrument features closed case electronic calibration. No internal mechanical adjustments are required. The instrument calculates correction factors based upon an input reference value and stores the correction factors in non-volatile memory. This procedure demonstrates making the zero adjustment from the front panel. The gain adjustments are similar.

DO NOT perform this procedure before reading Chapter 4. Chapter 4 describes this procedure, the required input connections, input signals, and test considerations required for a valid adjustment.

Measure

1 Configure the channel.

You must configure a channel before applying performing the adjustment procedure. Configure the channel to DC VOLTS and 6½ digits.

2 Apply the input signal

In this example, the input signal is a copper short (*see page 66*).

Shift View

3 Setup the calibration.

The display will show **PERFORM CAL..**

View

4 Set the adjustment value.

The display will show the a number. Edit the number to the actual input value. For the Zero Adjustment, the input value is 0.000000.

+000.000,000 mVDC

View

5 Begin the adjustment.

The display will show the progress of the adjustment. When all the adjustments are completed, the display will show done.

DONE

To Apply Mx+B Scaling to Measurements

The scaling function allows you to apply a *gain* and *offset* to all readings on a specified multiplexer channel during a scan. In addition to setting the gain ("M") and offset ("B") values, you can also specify a custom measurement label for your scaled readings (RPM, PSI, etc.).

Measure

1 Configure the channel.

You must configure the channel (function, transducer type, etc.) before applying any scaling values. If you change the measurement configuration, scaling is turned off on that channel and the gain and offset values are reset (M=1 and B=0).

Mx+B

2 Set the gain and offset values.

The scaling values are stored in *non-volatile* memory for the specified channels. A Factory Reset turns off scaling and clears the scaling values on all channels. An Instrument Preset or Card Reset *does not* clear the scaling values and *does not* turn off scaling.

+1.000,000

Set Gain

-0.700,000 OHM

Set Offset

Mx+B

3 Select the custom label.

You can specify an optional three-character label for your scaled readings (RPM, PSI, etc.). The default label is the standard engineering unit for the selected function (VDC, OHM, etc.).

LABEL AS OHM

Scan

4 Scaling is now applied to the measurements.

To Read the Relay Cycle Count

The instrument has a relay maintenance system to help you predict relay end-of-life. The instrument counts every individual switch closure and stores the count in non-volatile memory on each module. You can query the total number of cycles on any channel. You can use this feature on any of the relay modules and the internal DMM.

- In addition to the channel relays, you can also query the count on backplane relays and bank relays. Note that you cannot control the state of these relays from the front panel but you can query the count.
- You can also query the state of the three relays on the internal DMM. These relays are numbered “1”, “2”, and “3”. These relays open or close each time a function or range is changed on a module.
- The HP 34908A multiplexer contains 40 channels which are switched (HI only) using only 20 relays. Each relay is used to switch HI on two different channels (and only one channel can be closed at a time). The channels are arranged such that channels 01 and 21 use different contacts on the same relay. The remaining channels are also paired in the same manner (channels 02 and 22, channels 03 and 23, etc.). Therefore, when you query the relay count on a channel, the number reflects the number of times that the relay was closed. For example, the relay count will always be the same on channels 01 and 21.
- For more information on relay life and load considerations, refer to “Relay Life and Preventative Maintenance” in the *HP 34970A User’s Guide*.
- To read the count on the active channel, choose the following item and then turn the knob. To read the count on the internal DMM relays, turn the knob counterclockwise beyond the lowest numbered channel in the instrument. To read the “hidden” relays, turn the knob clockwise beyond the highest numbered channel in the current slot.



RELAY CYCLES

To Read a Digital Input Port

The multifunction module (HP 34907A) has two non-isolated 8-bit input/output ports which you can use for reading digital patterns. You can read the live status of the bits on the port or you can configure a scan to include a digital read.





1 Select the Digital Input port.

Select the slot containing the multifunction module and continue turning the knob until DIN is displayed (channel 01 or 02).




2 Read the specified port.

You can specify whether you want to use binary or decimal format. Once you have selected the number base, it is used for all input or output operations on the same port. To change the number base, press the  key and select USE BINARY or USE DECIMAL.

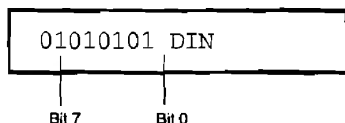

Binary Display Shown

The bit pattern read from the port will be displayed until you press another key, turn the knob, or until the display times out.

Note: To add a digital input channel to a scan list, press  and select the DIO READ choice.

To Write to a Digital Output Port

The multifunction module (HP 34907A) has two non-isolated 8-bit input/output ports which you can use for outputting digital patterns.




1 Select the Digital Output port.

Select the slot containing the multifunction module and continue turning the knob until DIN is displayed (channel 01 or 02).




2 Enter the bit pattern editor.


Notice that the port is now converted to an output port (DOUT).

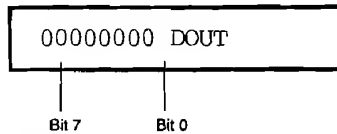

Binary Display Shown

3 Edit the bit pattern.

Use the knob and ◀ or ▶ keys to edit the individual bit values. You can specify whether you want to use binary or decimal format. Once you have selected the number base, it is used for all input or output operations on the same port. To change the number base, press the  key and select USE BINARY or USE DECIMAL.



Decimal Display Shown



4 Output the bit pattern to the specified port.

The specified bit pattern is latched on the specified port. To cancel an output operation in progress, wait for the display to time out.

To Read the Totalizer Count

The multifunction module (HP 34907A) has a 26-bit totalizer which can count TTL pulses at a 100 kHz rate. You can manually read the totalizer count or you can configure a scan to read the count.



1 Select the totalizer channel.

Select the slot containing the multifunction module and continue turning the knob until TOTALIZE (channel 03) is displayed.




2 Configure the totalize mode.

The internal count starts as soon as you turn on the instrument. You can configure the totalizer to reset the count to "0" after being read or it can count continuously and be manually reset.


READ + RESET




3 Read the count.

The count is read once each time you press ; the count does not update automatically on the display. As configured in this example, the count is automatically reset to "0" each time you read it.

12345 TOT

The count will be displayed until you press another key, turn the knob, or until the display times out. To manually reset the totalizer count, press .

Note: To add a totalizer channel to a scan list, press  and select the TOT READ choice.

To Output a DC Voltage

The multifunction module (HP 34907A) has two analog outputs capable of outputting calibrated voltages between ± 12 volts.



1 Select a DAC Output channel.

Select the slot containing the multifunction module and continue turning the knob until DAC is displayed (channel 04 or 05).



2 Enter the output voltage editor.

+00.000 V DAC


3 Set the desired output voltage.

Use the knob and ◀ or ▶ keys to edit the individual digits.

+05.250 V DAC



4 Output the voltage from the selected DAC.

The output voltage will be displayed until you press another key or turn the knob. To manually reset the output voltage to 0 volts, press .

Calibration Procedures

Calibration Procedures

This chapter contains procedures for verification of the instrument's performance and adjustment (calibration). The chapter is divided into the following sections:

- Hewlett-Packard Calibration Services, *on page 63*
- Calibration Interval, *on page 63*
- Time Required for Calibration, *on page 64*
- Automating Calibration Procedures, *on page 64*
- Recommended Test Equipment, *on page 65*
- Input connections, *on page 66*
- Calibration Security, *on page 67*
- Calibration Message, *on page 69*
- Calibration Count, *on page 69*
- Calibration Procedures, *on page 70*
- Aborting a Calibration in Progress, *on page 70*
- Test Considerations, *on page 71*
- Performance Verification Tests, *on page 72*
- Internal DMM Verification Tests, *on page 75*
- Optional AC Performance Verification Tests, *on page 80*
- Internal DMM Adjustments, *on page 81*
- -10 Vdc Adjustment Procedure (Optional), *on page 85*
- Plug-in Module Test Considerations, *on page 87*
- Relay Verification, *on page 88*
- Thermocouple Reference Junction, *on page 94*
- HP 34907A Analog Output, *on page 96*

Closed-Case Electronic Calibration The instrument features closed-case electronic calibration. No internal mechanical adjustments are required. The instrument calculates correction factors based upon the input reference value you set. The new correction factors are stored in non-volatile memory until the next calibration adjustment is performed. Non-volatile EEPROM calibration memory does not change when power has been off or after a remote interface reset.

Hewlett-Packard Calibration Services

When your instrument is due for calibration, contact your local Hewlett-Packard Service Center for a low-cost recalibration. The HP 34970A is supported on automated calibration systems which allow Hewlett-Packard to provide this service at competitive prices.

Calibration Interval

The instrument should be calibrated on a regular interval determined by the measurement accuracy requirements of your application. A 1-year interval is adequate for most applications. Accuracy specifications are warranted *only* if adjustment is made at regular calibration intervals. Accuracy specifications are not warranted beyond the 1-year calibration interval. Hewlett-Packard does not recommend extending calibration intervals beyond 2 years for any application.

Adjustment is recommended

Whatever calibration interval you select, Hewlett-Packard recommends that *complete re-adjustment should always be performed* at the calibration interval. This will assure that the HP 34970A will remain within specification for the next calibration interval. This criteria for re-adjustment provides the best long-term stability. Performance data measured using this method *can* be used to extend future calibration intervals.

Use the Calibration Count (*see page 69*) to verify that all adjustments have been performed.

Time Required for Calibration

The HP 34970A can be automatically calibrated under computer control. With computer control you can perform the complete calibration procedure and performance verification tests in less than 30 minutes once the instrument is warmed-up (see *“Test Considerations” on page 71*). Manual calibrations using the recommended test equipment will take approximately 2 hours.

Automating Calibration Procedures

You can automate the complete verification and adjustment procedures outlined in this chapter if you have access to programmable test equipment. You can program the instrument configurations specified for each test over the remote interface. You can then enter readback verification data into a test program and compare the results to the appropriate test limit values.

You can also adjust the instrument from the remote interface. Remote adjustment is similar to the local front-panel procedure. You can use a computer to perform the adjustment by first selecting the required function and range. The calibration value is sent to the instrument and then the calibration is initiated over the remote interface. The instrument must be unsecured prior to initiating the calibration procedure.

For further information on programming the instrument, see chapter 5 in the *HP 34970A User's Guide*.

Recommended Test Equipment

The test equipment recommended for the performance verification and adjustment procedures is listed below. If the exact instrument is not available, substitute calibration standards of equivalent accuracy.

A suggested alternate method would be to use the HP 3458A 8½ digit Digital Multimeter to measure less accurate yet stable sources. The output value measured from the source can be entered into the instrument as the target calibration value.


Application	Recommended Equipment	Accuracy Requirements
Zero Calibration ^[1]	None	4 -terminal all copper short
DC Voltage ^[1]	Fluke 5700A	<1/5 instrument 24 hour spec
DC Current ^[1]	Fluke 5700A/ 5725A	<1/5 instrument 24 hour spec
Resistance ^[1]	Fluke 5700A	<1/5 instrument 24 hour spec
AC Voltage ^[1]	Fluke 5700A/ 5725A	<1/5 instrument 24 hour spec
AC Current ^[1]	Fluke 5700A/ 5725A	<1/5 instrument 24 hour spec
Frequency ^[1]	HP 33120A	<1/5 instrument 24 hour spec
Analog Output HP 34907A	HP 34401A	<1/5 instrument 24 hour spec
Thermocouple Reference Junction HP 34901A HP 34902A HP 34908A	Thermistor YSI 44031 (two) J Type Calibrated Thermocouple Triple Point Cell	± 0.1 °C
Relay contact resistance All switch modules	HP 34401A	0.001 Ω resolution

[1] In addition to the internal DMM, these applications require an input multiplexer module. The HP 34901A is recommended.

Input Connections

You will need an input multiplexer module to verify or adjust the internal DMM. Input connections can be made using an HP 34901A 20-Channel Multiplexer.

To use an HP 34901A to completely verify and adjust the internal DMM, make the following connections:

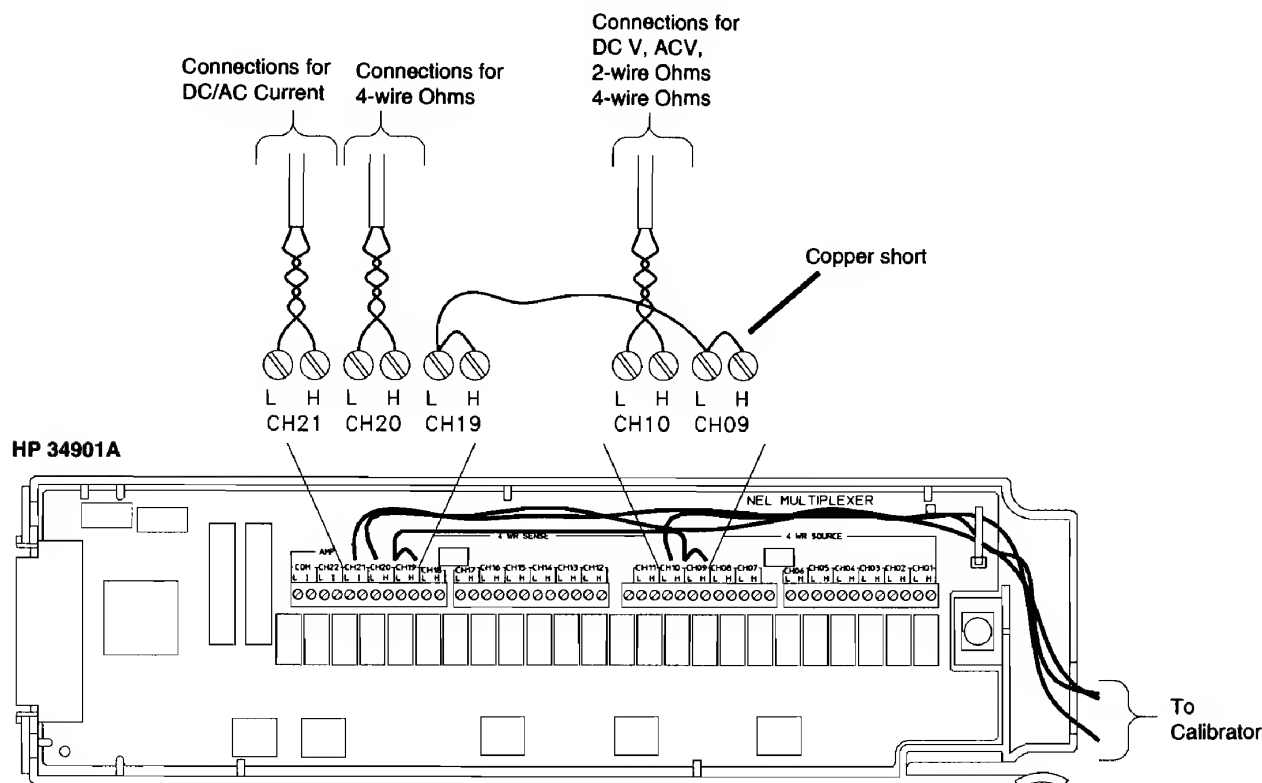

Note: Use shielded twisted pair Teflon[®] insulated cables to reduce settling and noise errors. Connect the shield to the source LO output.

You can also use an HP 34902A for test and adjustment of voltage, frequency, and resistance functions. You cannot test or adjust current inputs with an HP 34902A. If you use an HP 34902A; connect the copper shorts to channels 7 and 15 and make the input connections to channels 8 and 16.

Teflon[®] is a registered trademark of E.I. du Pont de Nemours and Company

Calibration Security

This feature allows you to enter a security code to prevent accidental or unauthorized adjustments of the instrument. When you first receive your instrument, it is secured. Before you can adjust the instrument, you must unsecure it by entering the correct security code. *See page 51 in Chapter 3 for a procedure to enter the security code.*


- The security code is set to “HP034970” when the instrument is shipped from the factory. The security code is stored in *non-volatile* memory, and *does not* change when power has been off, after a Factory Reset (*RST command), or after an Instrument Preset (SYSTem:PRESet command).
- The security code may contain up to 12 alphanumeric characters. The first character *must* be a letter, but the remaining characters can be letters, numbers, or an underscore (_). You do not have to use all 12 characters but the first character must always be a letter.

Note: *If you forget your security code, you can disable the security feature by adding a jumper inside the instrument as described on the following page.*

To Unsecure the Instrument Without the Security Code

To unsecure the instrument without the correct security code, follow the steps below. A front panel procedure to unsecure the instrument is given on page 51. See *“Electrostatic Discharge (ESD) Precautions”* on page 144 before beginning this procedure.

- 1 Disconnect the power cord and all input connections.
- 2 Remove the instrument cover. *Refer to page 156.* Turn the instrument over.
- 3 Apply power and turn on the instrument.
Be careful not to touch the power line connections.
- 4 Apply a short between the two exposed metal pads marked CAL UNLOCK as shown in the figure below.

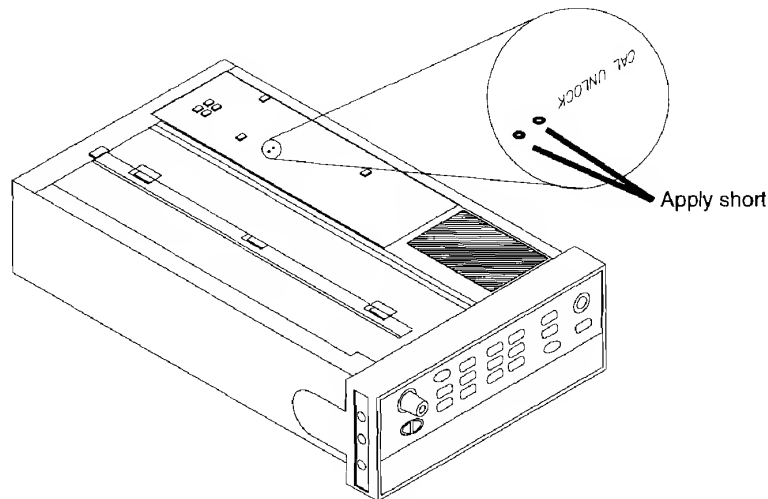

- 5 While maintaining the short, enter any unsecure code.
The instrument is now unsecured.
- 6 Remove the short.
- 7 Turn off the instrument and remove the power cord. Reassemble the instrument.

Now you can enter a new security code. Be sure you take note of the new security code.

Warning



- Exposed Mains
- Do Not Touch

Calibration Message

The instrument allows you to store one message in calibration memory. For example, you can store such information as the date when the last calibration was performed, the date when the next calibration is due, the instrument's serial number, or even the name and phone number of the person to contact for a new calibration.

You can record a calibration message *only* from the remote interface and *only* when the instrument is unsecured. You can read the message from either the front-panel or over the remote interface. You can read the calibration message whether the instrument is secured or unsecured.

- The calibration message may contain up to 40 characters. From the front panel, you can view 13 characters of the message at a time.

Press  to scroll through the text of the message. Press  again to increase the scrolling speed.

Calibration Count

You can query the instrument to determine how many calibrations have been performed. Note that your instrument was calibrated before it left the factory. When you receive your instrument, be sure to read the count to determine its initial value.

- The calibration count increments up to a maximum of 65,535 after which it resets to 0. Since the value increments by one for each calibration point, a complete calibration may increase the value by many counts.

Calibration Procedure

The following procedure is the recommended method to complete an instrument calibration.

- 1 Read “Test Considerations” (*page 71*).
- 2 Unsecure the instrument for calibration (*page 51*).
- 3 Perform the *verification* tests to characterize the instrument (incoming data).
- 4 Perform the zero *adjustment* procedures.
- 5 Perform the gain *adjustment* procedures. Perform the *verification* tests to verify the adjustments (outgoing data).
- 6 Secure the instrument against calibration.
- 7 Note the new security code and calibration count in the instrument’s maintenance records.

Aborting a Calibration in Progress

Sometimes it may be necessary to abort a calibration after the procedure has already been initiated. You can abort a calibration at any time by turning off the power. When performing a calibration from the remote interface, you can abort a calibration by issuing a remote interface device clear message.

CAUTION

If you abort a calibration in progress when the instrument is attempting to write new calibration constants to EEPROM, you may lose all calibration constants for the function. Typically, upon re-applying power, the instrument will report error **705** ***Cal:Aborted***. You may also generate errors 740 through 746. If this occurs, you should not use the instrument until a complete re-adjustment has been performed.

Test Considerations

To ensure proper instrument operation, verify that you have selected the correct power line voltage prior to attempting any procedure in this chapter. See *"If the Instrument Does Not Turn On"*, on page 42.

Errors may be induced by ac signals present on the input leads during a self-test. Long test leads can also act as an antenna causing pick-up of ac signals.

For optimum performance, all procedures should comply with the following recommendations:

- Assure that the calibration ambient temperature is stable and between 18 °C and 28 °C. Ideally the calibration should be performed at 23 °C \pm 1 °C.
- Assure ambient relative humidity is less than 50%.
- Allow a 2-hour warm-up period with a copper short connected and the multiplexer module installed before verification or adjustment. The connections are shown in the figure on page 66.
- Use shielded twisted pair Teflon® insulated cables to reduce settling and noise errors. Keep the input cables as short as possible.
- Connect the input cable shield to the source LO output. Except where noted in the procedures, connect the calibrator LO source to earth ground.

2-wire Ohms measurements are affected by the entire path length, including the plug-in card trace length and slot trace lengths. On the HP 34901A, Channel 10 is recommended as the median path length (on the HP 34902A, use channel 8) for 2-wire Ohms verification and adjustments. Install the input multiplexer in slot 200.

Because the instrument is capable of making highly accurate measurements, you must take special care to ensure that the calibration standards and test procedures used do not introduce additional errors. Ideally, the standards used to verify and adjust the instrument should be an order of magnitude more accurate than each instrument range full scale error specification.

For the dc voltage, dc current, and resistance gain verification measurements, you should take care to ensure the calibrator's "0" output is correct. If necessary, the measurements can be referenced to the calibrator's "0" output using $Mx + B$ scaling (see page 54). You will need to set the offset for each range of the measuring function being verified.

Performance Verification Tests



Use the Performance verification Tests to verify the measurement performance of the instrument. The performance verification tests use the instrument's specifications listed in chapter 1, "Specifications," starting on page 15.

You can perform four different levels of performance verification tests:

- **Self-Test** A series of internal verification tests that give a high confidence that the instrument is operational.
- **Quick Verification** A combination of the internal self-tests and selected verification tests.
- **Performance Verification Tests** An extensive set of tests that are recommended as an acceptance test when you first receive the instrument or after performing adjustments.
- **Optional Verification Tests** Tests *not* performed with every calibration. Perform these tests to verify additional specifications or functions of the instrument.

Self-Test

A brief power-on self-test occurs automatically whenever you turn on the instrument. This limited test assures that the instrument is capable of operation and also checks the plug-in cards for basic operation.

To perform a complete self-test hold down the  key as you press the power switch to turn on the instrument; *hold down the  key for more than 5 seconds until the instrument beeps* (a complete description of these tests can be found in chapter 6). The instrument will automatically perform the complete self-test procedure when you release the key. The self-test will complete in *approximately 20 seconds*.

- If the self-test is successful, “PASS” is displayed on the front panel.
- If the self-test fails, “FAIL” is displayed and the **ERROR** annunciator turns on. If repair is required, see chapter 6, “Service,” for further details.
- If all tests pass, you have a high confidence ($\approx 90\%$) that the instrument is operational.

Quick Performance Check

The quick performance check is a combination of internal self-test and an abbreviated performance test (specified by the letter **Q** in the performance verification tests). This test provides a simple method to achieve high confidence in the instrument's ability to functionally operate and meet specifications. These tests represent the absolute minimum set of performance checks recommended following any service activity. Auditing the instrument's performance for the quick check points (designated by a **Q**) verifies performance for "normal" accuracy drift mechanisms. *This test does not check for abnormal component failures.*

To perform the quick performance check, do the following:

- Perform a complete self-test. A procedure is given on page 73.
- Perform only the performance verification tests indicated with the letter **Q**.

If the instrument fails the quick performance check, adjustment or repair is required.

Performance Verification Tests

The performance verification tests are recommended as acceptance tests when you first receive the instrument. The acceptance test results should be compared against the 90 day test limits. You should use the 24-hour test limits only for verification within 24 hours after performing the adjustment procedure. After acceptance, you should repeat the performance verification tests at every calibration interval.

If the instrument fails performance verification, adjustment or repair is required.

Adjustment is recommended at every calibration interval. If adjustment is not made, you must guard band, using no more than 80% of the specifications listed in Chapter 1, as the verification limits.

Internal DMM Verification Tests

These procedures use inputs connected to an HP 34901A 20-Channel Multiplexer (*see page 66*) installed in slot 200.

Zero Offset Verification

This procedure is used to check the zero offset performance of the internal DMM. Verification checks are only performed for those functions and ranges with unique offset calibration constants. Measurements are checked for each function and range as described in the procedure below.

Zero Offset Verification Procedure

- 1 Make sure you have read “Test Considerations” on page 71.
- 2 This procedure will measure the shorts installed on channels 209 and 219. Leave the Amps input connections (channel 221) open.

Continued on the next page ...

Zero Offset Verification Procedure (Continued)

- 3 Select each function and range in the order shown in the table below. Before executing each test, you must press Mon to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface). Compare measurement results to the appropriate test limits shown in the table (see page 74).

Input	Channel 221		Quick Check	Error from Nominal		
	Function ^[1]	Range		24 hour	90 day	1 year
Open	DC Current	10 mA	Q	± 1 µA	± 2 µA	± 2 µA
Open		100 mA		± 4 µA	± 5 µA	± 5 µA
Open		1 A		± 60 µA	± 100 µA	± 100 µA
Input	Channel 209		Quick Check	Error from Nominal		
	Function ^[1]	Range		24 hour	90 day	1 year
Short	DC Volts	100 mV	Q	± 3.5 µV	± 4 µV	± 4 µV
Short		1 V		± 6 µV	± 7 µV	± 7 µV
Short		10 V		± 40 µV	± 50 µV	± 50 µV
Short		100 V		± 600 µV	± 600 µV	± 600 µV
Short		300 V		± 6 mV	± 9 mV	± 9 mV
Short	2-Wire Ohms ^[2] and 4-Wire Ohms	100 Ω	Q	± 3.5 mΩ	± 4 mΩ	± 4 mΩ
Short		1 kΩ		± 6 mΩ	± 10 mΩ	± 10 mΩ
Short		10 kΩ		± 50 mΩ	± 100 mΩ	± 100 mΩ
Short		100 kΩ		± 500 mΩ	± 1 Ω	± 1 Ω
Short		1 MΩ		± 10 Ω	± 10 Ω	± 10 Ω
Short		10 MΩ		± 100 Ω	± 100 Ω	± 100 Ω
Short		100 MΩ		± 10 kΩ	± 10 kΩ	± 10 kΩ

[1] Select 6½ digit resolution.

[2] For 2-wire ohms, an additional 1 Ω of error must be added. Also, see the note on page 71.


Q: Quick performance verification test points.

Note: Zero offset calibration using a multifunction calibrator is NOT recommended. The calibrator and cabling offset can be large and unstable causing poor offset calibration of the internal DMM.

Gain Verification

This procedure is used to check the “full scale” reading accuracy of the internal DMM. Verification checks are performed only for those functions and ranges with unique gain calibration constants. Begin verification by selecting a measuring function and range. *Make sure you have read “Test Considerations” on page 71.*

DC VOLTS, Resistance, and DC CURRENT Gain Verification Test

- 1 Make sure you have read “Test Considerations” on page 71.
- 2 Select each function and range in the order shown below.
Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface).
- 3 Compare measurement results to the appropriate test limits shown in the table. (Be certain to allow for appropriate source settling.)

Input	Channel 210		Quick Check	Error from Nominal		
	Function ^[1]	Range		24 hour	90 day	1 year
100 mV	DC Volts	100 mV	Q	± 6.5 µV	± 8 µV	± 9 µV
1 V		1 V		± 26 µV	± 37 µV	± 47 µV
10 V		10 V		± 190 µV	± 250 µV	± 400 µV
100 V		100 V		± 2.6 mV	± 4.1 mV	± 5.1 mV
300 V		300 V		± 12 mV	± 19.5 mV	± 22.5 mV
100 Ω	2-Wire Ohms ^[2] and 4-Wire Ohms	100 Ω	Q	± 6.5 mΩ	± 12 mΩ	± 14 mΩ
1 kΩ		1 kΩ		± 26 mΩ	± 90 mΩ	± 110 mΩ
10 kΩ		10 kΩ		± 250 mΩ	± 900 mΩ	± 1.1 Ω
100 kΩ		100 kΩ		± 2.5 Ω	± 9 Ω	± 11 Ω
1 MΩ		1 MΩ	Q	± 30 Ω	± 90 Ω	± 110 Ω
10 MΩ		10 MΩ		± 1.6 kΩ	± 2.1 kΩ	± 4.1 kΩ
100 MΩ ^[3]		100 MΩ		± 310 kΩ	± 801 kΩ	± 810 kΩ
Input	Channel 221		Quick Check	Error from Nominal		
	Function ^[1]	Range		24 hour	90 day	1 year
10 mA	DC Current	10 mA	Q	± 1.5 µA	± 5 µA	± 7 µA
100 mA		100 mA		± 14 µA	± 35 µA	± 55 µA
1 A		1 A		± 560 µA	± 900 µA	± 1.1 mA

[1] Select 6½ digit resolution.

[2] For 2-wire ohm an additional 1 Ω of error must be added. Also, see the note on page 71.

[3] Verify only, no adjustment required.


Q: Quick performance verification test points.

Chapter 4 Calibration Procedures

Internal DMM Verification Tests

AC VOLTS Gain Verification Test

Configuration: AC Volts
LF 3 HZ:SLOW (in the *Advanced* menu)

- 1 Make sure you have read "Test Considerations" on page 71.
- 2 Select channel 210, set the AC VOLTS function and the 3 Hz input filter. With the slow filter selected, each measurement takes 7 seconds to complete. Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface).
- 3 Select each range in the order shown below. Compare measurement results to the appropriate test limits shown in the table. (Be certain to allow for appropriate source settling.)

Input		Range	Quick Check	Error from Nominal		
V rms	Frequency			24 hours	30 days	1 year
100 mV	1 kHz	100 mV	Q	± 70 µV	± 90 µV	± 100 µV
100 mV	50 kHz	1		± 150 µV	± 160 µV	± 170 µV
1 V	1 kHz			± 700 µV	± 900 µV	± 1 mV
1 V	50 kHz	10 V	Q	± 1.5 mV	± 1.6 mV	± 1.7 mV
10 V	1 kHz			± 7 mV	± 13 mV	± 14 mV
10 V	50 kHz			± 14 mV	± 16 mV	± 17 mV
10 V	10 Hz			± 7 mV	± 13 mV	± 14 mV
10 mV ^[1]	1 kHz	100 mV	Q	± 34 µV	± 45 µV	± 46 µV
100 V	1 kHz	100 V		± 70 mV	± 90 mV	± 100 mV
100 V	50 kHz	300 V		± 150 mV	± 160 mV	± 170 mV
300 V	1 kHz			± 270 mV	± 390 mV	± 420 mV
300 V ^[2]	50 kHz			± 600 mV	± 690 mV	± 720 mV

[1] For this test, isolate the calibrator's output from earth ground.


[2] Some calibrators may have difficulty driving the internal DMM and cable load at this V-Hz output. Use short, low capacitance cable to reduce calibration loading. Verification can be performed at >195 Vrms. New test limits can be computed from the accuracy specification shown in Chapter 1 for the actual test conditions used.

Q: Quick performance verification test points.

Note: The 50 kHz ac voltage test points may fail performance verification if the internal shields have been removed and reinstalled. See "Gain Adjustment," on page 82, for further information on how to recalibrate the ac voltage function.

AC CURRENT Gain Verification Test

Configuration: AC Current
LF 3 HZ:SLOW (in the *Advanced* menu)

- 1 Make sure you have read "Test Considerations" on page 71.
- 2 Select channel 221, set the AC CURRENT function and the 3 Hz input filter. With the slow filter selected, each measurement takes 7 seconds to complete. Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTE:MON command from the remote interface).
- 3 Select each range in the order shown below. Compare measurement results to the appropriate test limits shown in the table.
(Be certain to allow for appropriate source settling.)

Input		Range	Quick check	Error from Nominal		
Current	Frequency			24 hour	90 day	1 year
10 mA ^[1]	1 kHz	10 mA	Q	± 14 µA	± 14 µA	± 14 µA
100 mA ^[1]	1 kHz	100 mA		± 600 µA	± 600 µA	± 600 µA
10 mA	1 kHz	1 A		± 510 µA	± 510 µA	± 510 µA
1A ^[1]	1 kHz	1A		± 1.4 mA	± 1.4 mA	± 1.4 mA

[1] Verify only, no adjustment.

Frequency Gain Verification Test

Configuration: Frequency
6½ digits

- 1 Make sure you have read "Test Considerations" on page 71.
- 2 Select channel 210, select the FREQUENCY function and set 6½ digits.
- 3 Select each range in the order shown below. Compare measurement results to the appropriate test limits shown in the table.
(Be certain to allow for appropriate source settling.)

Input		Range	Quick Check	Error from Nominal		
Voltage	Frequency			24 hour	90 day	1 year
10 mV ^[1]	100 Hz	100 mV	Q	± 0.06 Hz	± 0.1 Hz	± 0.1 Hz
1 V	100 kHz	1 V		± 6 Hz	± 10 Hz	± 10 Hz


[1] Verify only, No adjustment. For this test, isolate the calibrator's output from earth ground.

Q: Quick performance verification test points.

Optional AC Performance Verification Tests

These tests are *not* intended to be performed with every calibration. They are provided as an aid for verifying additional instrument specifications. There are *no adjustments* for these tests; they are provided for performance verification only.

Configuration: AC VOLTS
 LF 3 HZ:SLOW (in the *Advanced* menu)

- 1 Make sure you have read "Test Considerations" on page 71.
- 2 Select channel 210, select the AC Volts function and the 3 HZ filter. Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface).
- 3 Select each range in the order shown below. Compare measurement results to the appropriate test limits shown in the table. (Be certain to allow for appropriate source settling.)

Input		Range	Error from Nominal		
Voltage	Frequency		24 hour	90 day	1 year
1 V	20 Hz	1 V	±700 µV	±900 µV	±1 mV
1 V	20 kHz	1 V	±700 µV	±900 µV	±1 mV
1 V	100 kHz	1 V	±6.3 mV	±6.8 mV	±6.8 mV
1 V	300 kHz	1 V	±45 mV	±45 mV	±45 mV
10 V	1 kHz	10 V	±7 mV	±9 mV	±10 mV
1 V	1 kHz	10 V	±3.4 mV	±4.5 mV	±4.6 mV
100 mV	1 kHz	10 V	±13 mV	±14 mV	±14 mV

Internal DMM Adjustments

You will need an HP 34901A 20-Channel Multiplexer to perform the following procedures (see page 66) Install the Multiplexer in slot 200.

Zero Adjustment

Each time you perform a zero adjustment, the Internal DMM stores a new set of offset correction constants for every measurement function and range. The Internal DMM will sequence through all required functions and ranges automatically and store new zero offset calibration constants. All offset corrections are determined automatically. *You may not correct a single range or function without re-entering ALL zero offset correction constants automatically. This feature is intended to save calibration time and improve zero calibration consistency.*

Note: *Never turn off the Internal DMM during Zero Adjustment. This may cause ALL calibration memory to be lost.*

Zero Adjustment Procedure

The zero adjustment procedure takes about 5 minutes to complete. Be sure to allow the instrument to warm up for 2 hours before performing the adjustments.

Follow the steps outlined below. Review “Test Considerations” on page 71 before beginning this test. Also see page 53, for an example of how to initiate a zero calibration.

- 1 This procedure will use the copper shorts installed on channels 209 and 219. Leave the Amps input connections (channel 221) open.
- 2 Select channel 209. Select the DC VOLTS function.
- 3 Press **Shift** **View** to enter the calibration menu. Press **View** again to begin the adjustment procedure.
- 4 Use the knob and arrow keys to set the number in the display to 0.000000 and press **View**.
- 5 Perform the Zero Offset Verification tests (see page 75) to check zero calibration results.

Gain Adjustment

The Internal DMM stores a *single* new gain correction constant each time this procedure is followed. The gain constant is computed from the calibration value entered for the calibration command and from measurements made automatically during the adjustment procedure.

Most measuring functions and ranges have gain adjustment procedures. Only the 100 M Ω range *does not* have gain calibration procedures. The gain calibration value may be entered through the front panel menu or over the remote interface. See page 53, for an example of how to enter calibration values.

Adjustments for each function should be performed ONLY in the order shown in the performance verification table. See "Performance Verification Tests" earlier in this chapter for the tables used for gain adjustments.

Gain Adjustment Considerations

- The zero adjustment procedure *must* have been recently performed prior to beginning any gain adjustment procedures.
- The optional –10 Vdc adjustment should be performed *only* after servicing the Internal DMM's a-to-d converter or after replacing network A4U101 or calibration RAM A4U505.
- When performing a 4-wire ohms gain adjustment, a new gain correction constant is *also stored* for the corresponding 2-wire ohms measurement range. If desired, the 2-wire gain can be adjusted separately **after** the 4-wire ohms gain calibration is completed.
- During the ac voltage gain adjustments, some of the dc voltage gain constants are used. Perform the dc voltage gain calibration before the ac voltage gain calibration.

Note: *Never turn off the instrument during a Gain Adjustment. This may cause calibration memory for the present function to be lost.*

Valid Gain Adjustment Input Values

Gain adjustment can be accomplished using the following input values.

Function	Range	Valid Calibration Input Values
DC VOLTS	100 mV to 100 V 300 V	0.9 to 1.1 x Full Scale 250 V to 303 V
OHMS, OHMS 4W	100 Ω to 10 M Ω	0.9 to 1.1 x Full Scale
DC CURRENT	10 mA to 1 A	0.9 to 1.1 x Full Scale
AC VOLTS [1]	10 mV to 100 V 300 V	0.9 to 1.1 x Full Scale 95 V to 303 V
AC CURRENT	10 mA	9 mA to 11 mA
Frequency	Any	Any Input > 100 mV rms, 1 kHz ~ 100 kHz

[1] Valid frequencies are as follows: 1 kHz \pm 10% for the 1 kHz calibration,
45 kHz ~ 100 kHz for the 50 kHz calibration,
and 10 Hz \pm 10% for the 10 Hz calibration.

Gain Adjustment Procedure




Adjustment for each function should be performed **only** in the order shown in the performance verification table. The performance verification tables used for gain adjustments start on page 77.

Review the “Test Considerations” (page 71) and “Gain Adjustment Considerations” (page 82) sections before beginning this test.




Configuration: dc functions — 6½ digits
 ac functions — LF 3 HZ:SLOW (in the *Advanced* menu)

- 1 Select channel 210. Configure the channel to each function and range shown in the gain verification tables (*pages 75 – 79*) .
- 2 Apply the input signal shown in the “Input” column of the appropriate verification table.

Note: *Always complete tests in the same order as shown in the appropriate verification table.*

- 3 Press   to enter the calibration menu. Press  again to begin the adjustment procedure.











- 4 Use the knob,  and  to set the number in the display to the actual input value and press .
- 5 Perform the appropriate Gain Verification Test to check the calibration results.
- 6 Repeat steps 1 through 6 for each gain verification test point shown in the tables.

Note: *Each range in the gain adjustment procedure takes less than 20 seconds to complete.*

–10 Vdc Adjustment Procedure (Optional)

The –10 Vdc calibration electronically enhances the Internal DMM's a-to-d converter linearity characteristic. *This adjustment should ONLY be performed after servicing the a-to-d converter or replacement of the calibration RAM.*








You will need an HP 34901A 20-Channel Multiplexer to perform the following procedures (see page 66) Install the Multiplexer in slot 200.

- 1 If a zero calibration has not been performed recently, perform one before beginning this procedure (see page 81).
- 2 Select channel 210. Configure the channel as follows:
DC VOLTS
10 V range
6½ digits
INTEG 100 PLC (in the *Advanced* menu)
INPUT R > 10 G (in the *Advanced* menu)
Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTE:MON command from the remote interface).
- 3 Measure and note the voltage offset present at the end of the measurement cable by shorting the ends of the channel 210 measurement cable. Be sure to use a copper wire and allow enough time for the residual thermal offset to stabilize (usually about 1 minute).
- 4 Connect the input cable to the calibrator output and set the calibrator to output +10V. Allow enough settling time for any thermal offset voltages to stabilize (usually about 1 minute).
- 5 Perform a +10V dc gain calibration. Press   to enter the calibration menu. Press  again to begin the adjustment procedure.
- 6  Use the knob,  and  to set the number in the display to the sum of the calibrator output and the measured offset (from step 3) and press . For example, if the calibrator output is 10.001 volts and the measured offset is 10 µV, enter +10.001010 volts. When the adjustment finishes, verify that new readings fall within ±20 µV of the calibrator output plus the offset.

Continued on the next page ...

Chapter 4 Calibration Procedures
-10 Vdc Adjustment Procedure (Optional)

-10 Vdc Adjustment Procedure (Continued)

- 7 Reverse the cable connections to the calibrator to create a -10 Vdc voltage standard. You *must* physically reverse the cables. *DO NOT* switch the output polarity of the calibrator.
- 8 Perform a -10V DC gain calibration. Press   to enter the calibration menu. Press  again to begin the adjustment procedure. Be sure to allow time for thermal offsets to stabilize (usually about 1 minute).
-  9 Use the knob  and  to set the number in the display to the *difference* of the calibrator output and the measured offset (from step 3) and press . Using the previous example values, enter 10 μ V minus 10.001 volts or -10.000990 volts.
- 10 When the adjustment finishes, verify that new readings fall within $\pm 30 \mu$ V of the calibrator output minus the offset.

Plug-in Module Test Considerations

For optimum performance, all test procedures should comply with the following recommendations:

- Assure that the calibration ambient temperature is stable and between 18 °C and 28 °C. Ideally the calibration should be performed at 23 °C \pm 1 °C.
- Assure ambient relative humidity is less than 50%.
- Install the plug-in module and allow a 45 minute warm-up period before verification or adjustment.
- Use shielded twisted pair Teflon[®] insulated cables to reduce settling and noise errors. Keep the input cables as short as possible.
- Remove all user wiring and connections from the plug-in modules before verification or adjustment.
- Use 4-wire Ohms measurement techniques for checking relay contact resistance. Check directly at the terminals where possible.

Relay Verification

There are two methods you can use to verify relays:

- Read the relay cycle count.
- Measure the relay contact resistance.

Relay Cycle Count

The instrument has a relay maintenance system to help you predict relay end-of-life. The instrument counts every individual switch closure and stores the count in non-volatile memory on each module. You can query the total number of cycles on any channel. You can use this feature on any of the relay modules and the internal DMM.

- In addition to the channel relays, you can also query the count on backplane relays and bank relays. Note that you cannot control the state of these relays from the front panel but you can query the count.
- You can also query the state of the three relays on the internal DMM. These relays are numbered “1”, “2”, and “3”. These relays open or close when a function or range is changed on a module.
- The HP 34908A multiplexer contains 40 channels which are switched (HI only) using only 20 relays. Each relay is used to switch HI on two different channels (and only one channel can be closed at a time). The channels are arranged such that channels 01 and 21 use different contacts on the same relay. The remaining channels are also paired in the same manner (channels 02 and 22, channels 03 and 23, etc.). Therefore, when you query the relay count on a channel, the number reflects the number of times that the relay was closed. For example, the relay count will always be the same on channels 01 and 21.
- You can reset the count (allowed only from remote) but the instrument must be unsecured (see *“To Unsecure for Calibration”* on page 51 to unsecure the instrument).
- For more information on relay life and load considerations, refer to “Relay Life and Preventative Maintenance” in Chapter 8 of the *HP 34970A User’s Guide*.
- A procedure to read the relay cycle count is given on page 55.

HP 34901A Relay Contact Resistance Verification (Optional)


- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Install module in slot 100. Close channels 101 through 121. *See page 41.* Unplug the module.
- 3 Measure the following resistances:
 - CH01 H through CH11 H to COMMON SOURCE H
 - CH01 L through CH11 L to COMMON SOURCE L
 - CH12 H through CH20 H to COMMON SENSE H
 - CH12 L through CH20 L to COMMON SENSE L
 - CH21 H to AMPS COM H
 - CH21 L to AMPS COM L
 - CH22 H to CH12 L (bypass relay)
- 4 Install the module in slot 100. Close channel 122. Unplug the module.
- 5 Measure the following resistances:
 - CH22 H to AMPS COM H
 - CH22 L to AMPS COM L
 - CH21 H to CH21 L (bypass relay)

In general, a new relay should have a contact resistance of 1 Ω or less. Relays with contact resistance in excess of 2 Ω should be replaced.

HP 34902A Relay Contact Resistance Verification (Optional)

This procedure uses the internal DMM. Contact resistance verification with an external DMM is not recommended since the external COMMON terminals have a series 100 Ω protection resistor in each path.


- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Prepare the module by connecting a copper short from H to L on all 16 input channels. Do not short the COMMON terminals.
- 3 Connect a short jumper from pin 12 to pin 13 of J101 as shown.

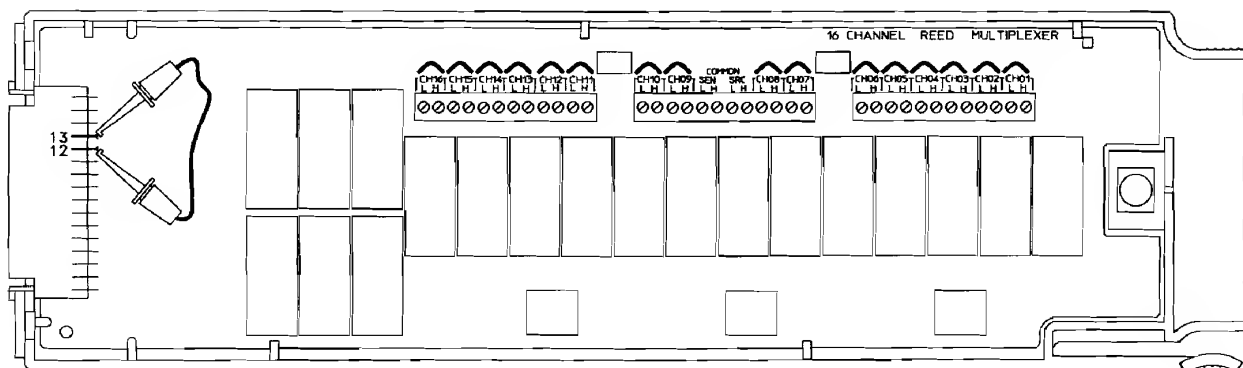

- 4 Install the module in slot 200. Select channel 201. Configure the channel as follows:
OHMS
100 OHM RANGE
6½ DIGITS
Before executing each test, you must press to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface).
- 5 Record the resistance shown in the display.

Continued on the next page ...

HP 34902A Relay Contact Resistance Verification (Continued)

- 6 Remove the module from the mainframe. Remove the jumper from J101.
- 7 Install the module in slot 200. Select channel 201. Configure the channel as follows:
OHMS
100 OHM RANGE
6½ DIGITS
Before executing each test, you must press  to enable reading monitoring on the selected channel (or use the ROUTE:MON command from the remote interface).
- 8 Subtract the displayed resistance measurement from the reference reading obtained step 4.
- 9 Repeat steps 6 and 7 for channel 202 through 216.

This procedure measures the resistance of 4 sets of relay contacts; the channel H and L and the backplane H and L. In general, the relay path should have a contact resistance of 1 Ω or less. Relay paths with contact resistance in excess of 1 Ω should be replaced.

HP 34903A Relay Contact Resistance Verification (Optional)

- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Install module in slot 100. Close channels 101 through 120. *See page 41.* Unplug the module.
- 3 Measure the resistance from the CM terminal to the NO terminal on each channel.
- 4 Install the module in slot 100. Open channel 101 through 120. Unplug the module.
- 5 Measure the resistance from the CM terminal to the NC terminal on each channel.

In general, a new relay should have a contact resistance of 1 Ω or less. Relays with contact resistance in excess of 2 Ω should be replaced.

HP 34904A Relay Contact Resistance Verification (Optional)

- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Install module in slot 100. Close channels 111 through 118. Verify all other channels are open. *See page 41.* Unplug the module.
- 3 Measure the following resistances:
 ROW 1 A to COL 1 A through COL 8 A
 ROW 1 B to COL 1 B through COL 8 B
- 4 Install the module in slot 100. Open channels 111 through 118. Close channel 121 through 128. Unplug the module.
- 5 Repeat step 4, measuring from the Row 2 A and B terminals.
- 6 Repeat steps 5, 6, and 7 for ROW 3 and ROW 4.

In general, a new relay should have a contact resistance of 1 Ω or less. Relays with contact resistance in excess of 2 Ω should be replaced.

HP 34905A/06A Relay Contact Resistance Verification (Optional)


Note: Be sure to use the correct SMB connectors (50 Ω or 75 Ω).

- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Prepare the module by connecting an SMB short to CH10, CH11, CH12, and CH13. Connect the COM1 terminal to the DMM. Be sure to use the correct SMB connectors for the module.
- 3 Install the module in slot 100.
- 4 Close channel 111.
- 5 Measure the resistance on the DMM.
- 6 Repeat steps 4 and 5 for channels 112, 113, and 114.
- 7 Repeat steps 2, 3, 4, 5, and 6 for the channels connected to COM2.

In general, a new relay should have a contact resistance of 1 Ω or less. Relays with contact resistance in excess of 2 Ω should be replaced.

HP 34908A Relay Contact Resistance Verification (Optional)

- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Prepare the module by connecting a copper short from H to H on all 40 input channels. Connect the DMM test leads from the COM H to Channel 11 H.

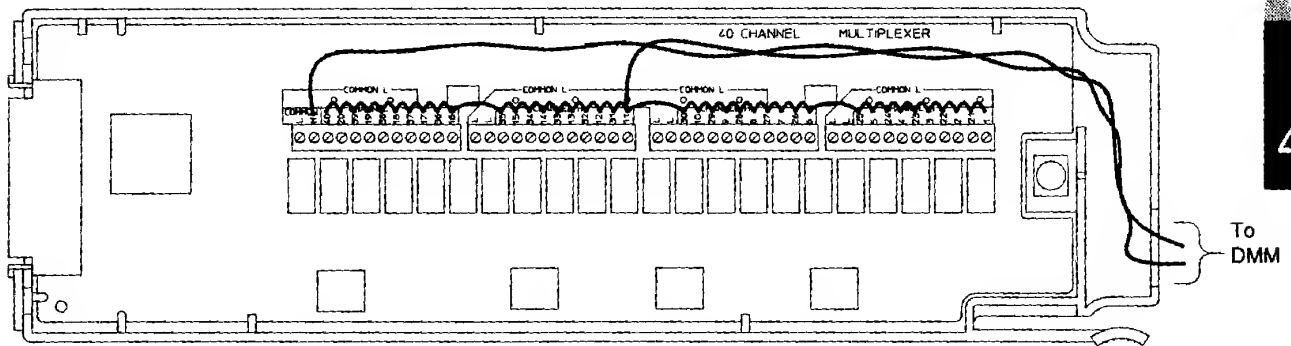

- 3 Install the module in slot 100.
- 4 Close channel 101. Measure the resistance on the DMM.
- 5 Repeat step 4 for channels 102 through 140.

This procedure measures the resistance of 2 sets of relay contacts; the channel H and the tree switch H. In general, a new relay should have a contact resistance of 1 Ω or less. Relays with contact resistance in excess of 2 Ω should be replaced.

Thermocouple Reference Junction (Optional)

Note: You should perform these verification and adjustments if you are using the modules for thermocouple measurements.

To make a thermocouple measurement a known reference junction temperature measurement must be made. The reference junction temperature is measured by two solid state temperature sensors in the input connection area on the module. The adjustments store calibration constants used to correct the measurements from the temperature sensors.

Thermocouple measurements are only supported by the HP 34901A, HP 34902A and HP 34908A.

Thermocouple Reference Junction Verification

- 1 Read "Plug-in Module Test Considerations" on page 87.
- 2 Connect a calibrated thermocouple to one of the following channels:

For the HP 34901A	Channel 10
For the HP 34902A	Channel 8
For the HP 34908A	Channel 10

Install the module in slot 100.
- 3 Place the J Type calibrated thermocouple at a known temperature (ice bath or calibrator).
- 4 Select channel 110 (or 108). Configure the channel as follows:


TEMPERATURE
THERMOCOUPLE
J TYPE
INTEG 10 PLC (*Advanced* menu)
INTERNAL REF (*Advanced* menu)

Before executing each test, you must press Mon to enable reading monitoring on the selected channel (or use the ROUTe:MON command from the remote interface).
- 5 Subtract the thermocouple error from the displayed temperature. Verify the result is within ± 1.0 °C of the known temperature (set in step 3).

Thermocouple Reference Junction Adjustments

These adjustments are plug-in module specific and only affect thermocouple measurements. The calibration constants created by these adjustments are stored in non-volatile memory *on the plug-in module*.

- 1 Connect a 10 k Ω (YSI 44031) thermistor to each of the following channels:
 For the HP 34901A Channels 6 and 17
 For the HP 34902A Channels 6 and 11
 For the HP 34908A Channels 6 and 16
 Keep the thermistor leads as short as possible. Locate the thermistor as near to the input connectors as possible.

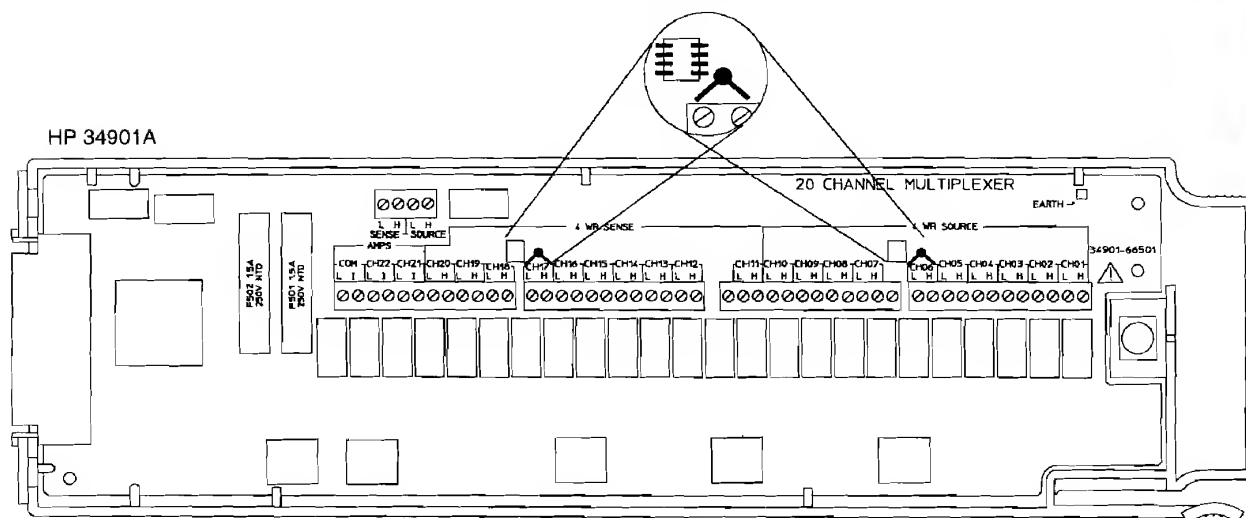


- 2 Install the plug-in module in the mainframe in slot 200. Apply power and allow a 2 hour warm-up.
- 3 Set 10 k Ω thermistor measurements on channels 206 and 217 (or 206 and 211). Before executing each test, you must press **Mon** to enable reading monitoring on the selected channel (or use the ROUTE:MON command from the remote interface).
- 4 Press **Shift View** to enter the calibration menu. Press **View** again to begin the adjustment procedure.
- 5 Verify the adjustment (see page 94).

HP 34907A Analog Output

Analog Output Verification Test

This procedure is used to check the calibration of the analog outputs on the HP 34907A Multifunction Module. Install the module in slot 200. Verification checks are performed only for those output values with unique calibration constants.

- 1 Make connections to analog output channels as shown below.

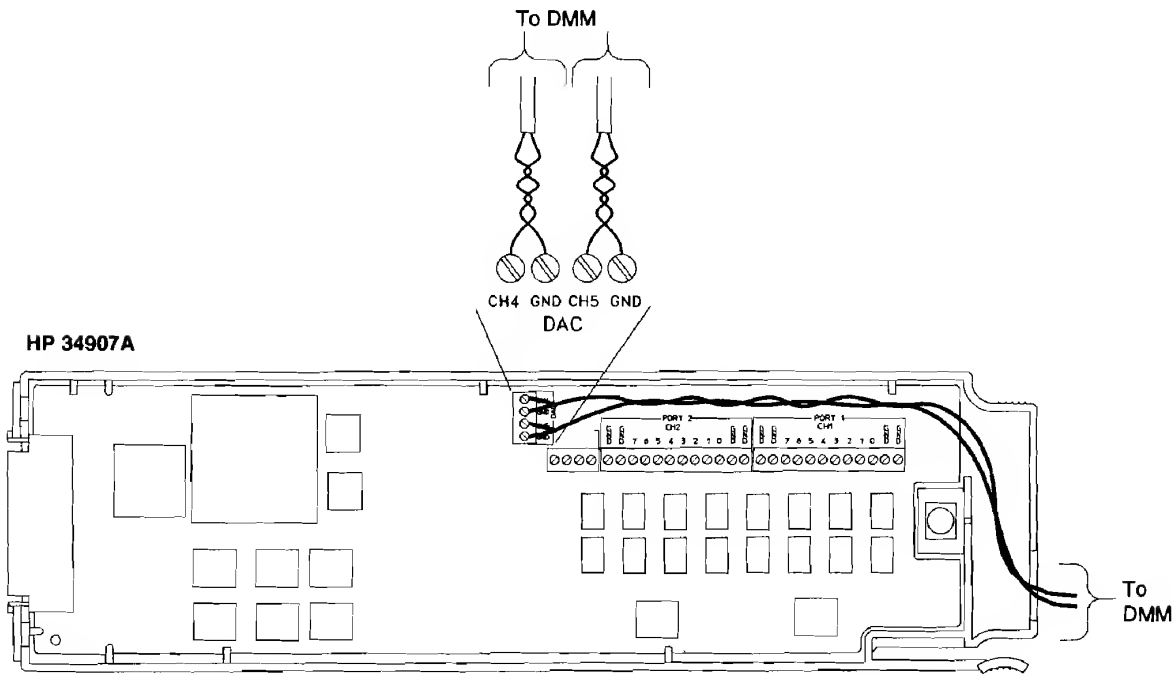















- 2 For each analog output, set each output value in the table below. Compare measurement results to the appropriate test limits shown in the table.

DAC Output	Quick Check	Measured Output	Error from Nominal		
			24 hour	90 day	1 year
0.000 V	Q	0.000 V	± 4 mV	± 6 mV	± 6 mV
10.000 V		10.000 V	± 8 mV	± 16 mV	± 21 mV

Analog Output Adjustment

Note: Install the HP34907A module in the mainframe and allow a 45 minute warm-up before performing these procedures.

This adjustment procedure sets a zero adjustment and a gain adjustment constant for each DAC output. You *must* perform all the adjustments on one analog output channel before adjusting the other analog output channel.

- 1 Install the module in slot 100.
Select the first analog output channel (104).
- 2 Connect an external DMM to the output terminals.
- 3 Set the analog output to 0.0000 V.
- 4 Press   to enter the calibration menu. Press  again to begin the adjustment procedure.
-  5 Use the knob  and  to set the number in the display to the measured output value and press  to complete the adjustment.
- 6 Set the analog output to 10.0000 V.
- 7 Press   to enter the calibration menu. Press  again to begin the adjustment procedure.
-  8 Use the knob,  and  to set the number in the display to the measured output value and press  to complete the adjustment.
- 9 Repeat steps 1 through 8 for channel 105.
- 10 Perform the Voltage Output Verification Test on page 96 to verify the adjustment.

Theory of Operation

Theory of Operation


This chapter is organized to provide descriptions of the circuitry contained on each schematic shown in chapter 9. A block diagram overview is provided followed by more detailed descriptions of the circuitry contained in the schematics chapter.

- System Block Diagram, *on page 101*
- Floating Logic, *on page 102*
- Memory, *on page 105*
- Earth-Referenced Logic, *on page 106*
- Power Supplies, *on page 107*
- Front Panel, *on page 109*
- Internal DMM, *on page 111*
- Switch Modules, *on page 120*
- Multifunction Module, *on page 133*

The self-test procedures are described in chapter 6.

System Block Diagram

A simplified block diagram is shown below. A detailed system block diagram is shown on page 205. Not all systems have an Internal DMM. In these systems, the internal DMM connections to the analog bus and the floating logic are left open. The major portions of each block are described in the following sections.

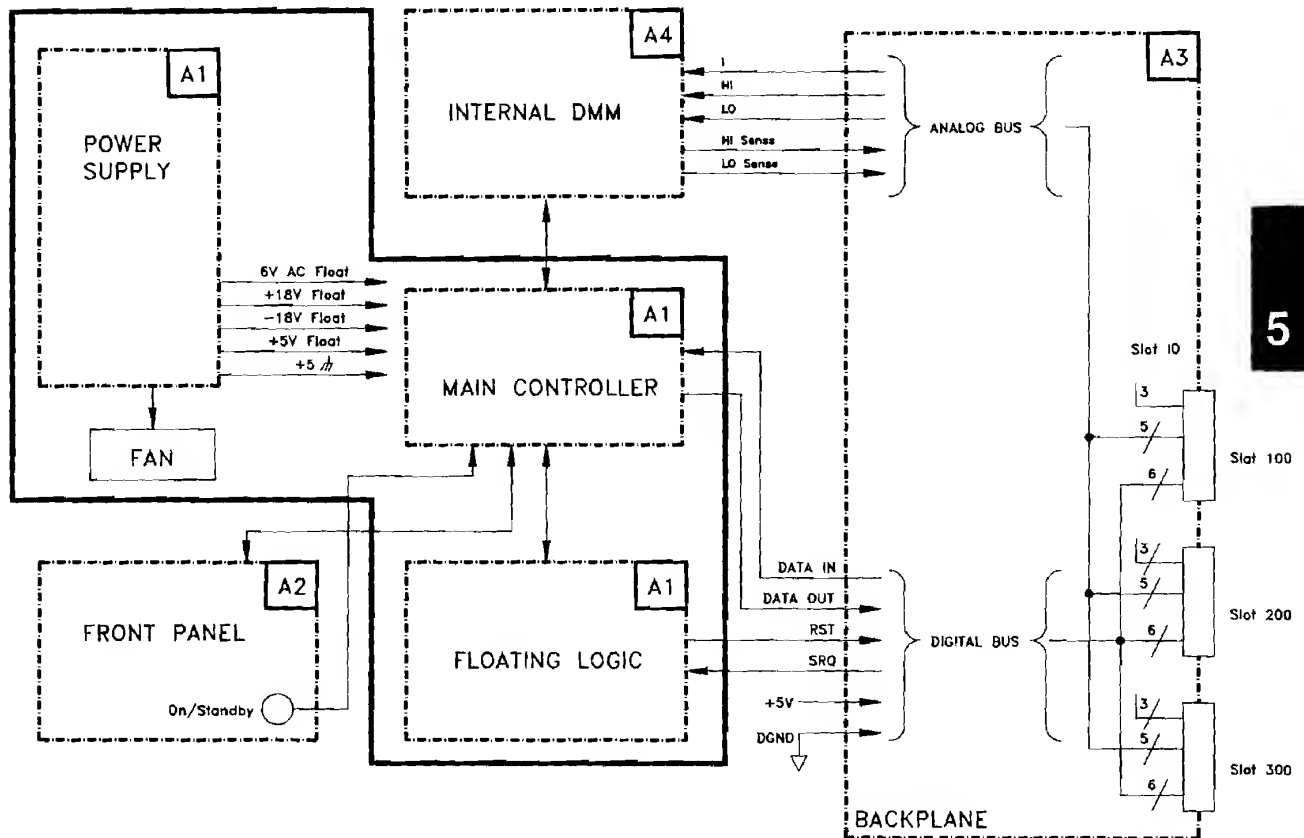

Floating Logic

Unless otherwise noted, components in this discussion are located on the A1 circuit assembly (34970-66501). The schematics begin on page 208.

The floating common logic controls the operation of the entire instrument. All measurement control and remote interface command interpretation is performed in the main controller, U205. The front panel controller, the I/O controller, and all of the plug-in module controllers, act as slaves to U205. The floating common logic is comprised of the main controller U205, custom ASIC U209, calibration memory U201, 12 Mhz clock oscillator U204, and microprocessor supervisor U104.

The microprocessor supervisor U104 performs the following functions:

- Monitors the regulated 5V floating supply and generates the reset signal for main controller U205 when the voltage drops below operating levels.
- Monitors the unregulated side of the 5V floating supply in order to generate an early warning signal (PWRFAIL) when power is lost.
- Provides automatic switch over to the battery BT101 for the +5V_NV supply when the 5V_FLT supply drops below the battery voltage.
- Blocks the main controller's write signal (WR_N) while the 5V_FLT supply is below operating level.

The main controller, U205, is a 16-bit microcontroller incorporating many built-in features:

- A 10-bit, successive approximation ADC with selectable inputs is used to convert two signals: FLASH and FRQRNG. The FLASH signal is the residual charge on the main integrating ADC output from the internal DMM assembly (A4). The FRQRNG signal (also from the internal DMM) is used to make voltage ranging decisions for frequency and period measurements.
- A pulse-width-modulation port, after filtering the 23 kHz output with R221, C224, and R259, produces DC voltages between 0V and 5V. This voltage, PREADJ, is used to adjust the precharge amplifier offset voltage in U101 on the internal DMM assembly (A4).
- A full, UART controlled, serial port is used to communicate with the I/O processor through optoisolators U303 and U214. Data is sent in an 11-bit frame at a rate of 187.5 kbits/second. The 11-bit frame is configured for one start bit, nine data bits, and one stop bit.
- A timer is used to measure the power line frequency on LSENSE. Frequencies between 55 Hz and 66 Hz result in the use of a 60 Hz standard for the DMM integration period. All other frequencies will result in the use of a 50 Hz standard.
- A 16-bit counter counts pulses on CNT to create, along with the 8-bit counter in U209, a 24-bit counter for the internal DMM.

The custom ASIC, U209, provides:

- **Memory Address mapping** — The main controller multiplexes address and data on the same bus. U209 latches the address and drives a separate memory address bus (MA(19:1)). U209 allows the main controller to access a much larger memory space than its 16-bit address bus would allow. It also partitions memory into separate data and instruction segments and a “mappable” segment that can be used for either data or instructions.
- **Communications** — U209 provides three serial communication ports. A 187.5 kbit/second, 9 data bit, UART for communicating with the isolated backplane (FLT_BPDO and FLT_BPDI_N). A duplicate, 9-bit UART to communicate with the front panel (FPDO and FPDI). And a simple, 1.5 Mbit/second, clocked shift-register to control the configuration registers on the DMM assembly (CFG_SCK, CFG_DO, and CFG_DI).
- **Real Time Clock** — U209 provides time of day and date, a periodic interrupt, and a squarewave generator. The date is based on a 100 year calendar (it accurately tracks leap years until its two digit year counter rolls over). U209 uses the battery-backed +5V_NV supply.
- **DMM support** — U209 provides conversion logic for the analog-to-digital converter and a counter for both the ADC and the frequency measurement features of the DMM. When used for the ADC, the COMP input functions both as a clocked comparator and the slope counter input. When used for frequency measurement, FREQIN is the input to the counter. In both cases, the 8-bit counter produces the lower bits of a 24-bit counter. The counter overflow signal, CNT, is counted by U205 to produce the upper 16-bits of the count. The SYNC signal produced by U205, is used to latch the count.

Device U201 is a 512 byte, ferroelectric RAM that is accessed via a serial interface. This device only contains data relevant to the A1 assembly. This data is combined with data retrieved from A4U450 to completely calibrate the internal DMM. The two devices, although on different assemblies, share the same I/O signals, CALSCK and CALDAT, that allow them to be read (and written) by U205.

Memory

Unless otherwise noted, components in this discussion are located on the A1 circuit assembly (34970-66501). The schematics begin on page 208.

The main controller, U205, uses 512 Kbytes of ROM and 544 Kbytes of RAM. ASIC U209 provides the memory mapping that allows access to this large memory space. The memory map as seen by the main controller is as follows:

Address	Maps to
0100H thru 1FBFH	00100H thru 01FBFH in RAM for data fetches
0100H thru 1FBFH	00100H thru 01FBFH in ROM for instr. fetches
1FC0H thru 1DFDH	registers in U209
2000H thru 5FFFH	02000H thru 05FFFH in ROM
6000H thru 7FFFH	06000H thru 07FFFH in RAM for data fetches
6000H thru 7FFFH	06000H thru 07FFFH in ROM for instr. fetches
8000H thru FFFFH	any selected 32 Kbyte page of ROM or RAM

The memory is organized with a 16-bit data bus (AD(15:0)) and a 19-bit address bus (MA(19:1)). The memory address is produced by U209 latching the address present on AD(15:0) when U205 asserts ALE_FLT. Reads of memory are always 16-bits wide (there is a single RD_N signal). Writes, however, can be byte-wide and therefore U209 produces both a high-byte write strobe, MWRH_N, and a low-byte write strobe, MWRL_N. These write signals are based on the latched 0-bit of the address and the BHE_N signal produced by the main controller, U205.

The ROM memory consists of a single, 256Kx16 device, U401. The RAM memory consists of five devices: U402, U403, U404, U405, and U410. A uniform, 256Kx16, memory block is formed by the four 128Kx8 devices, U402 through U405. A separate, 32Kx8 block is formed by U410 and is available through special programming of U209.

Earth-Referenced Logic

Unless otherwise noted, components in this discussion are located on the A1 circuit assembly (34970-66501). The schematics begin on page 208.

The earth referenced logic circuits provide all rear panel input/output capability. Microprocessor U305 handles HP-IB (IEEE-488) control through bus interface chip U309 and bus receiver/driver chips U310 and U311.

The RS-232 interface is controlled by U305 through U307. RS-232 transceiver chip U308 provides the required level shifting to approximate ± 9 volt logic levels through on-chip charge-pump power supplies using capacitors C317 through C320. Communication between the earth referenced logic interface circuits and the floating measurement logic is accomplished through an optically-isolated bi-directional serial interface. Isolator U214 couples data from U305 to microprocessor U205. Isolator U303 couples data from U305 to microprocessor U205.

U305 also:

- Controls power to the backplane as well as all rear panel interfaces (HP-IB, RS-232, Alarms, External Triggers). Backplane power is turned on or off based upon commands received from U205.
- Drives the backplane reset signal (BPRST) based upon commands from U205.
- Monitors the backplane service request (BPSRQ_N) and reports to U205 when it is asserted.

U306B, U306C, U306D, and U306E drive the alarm outputs. The alarm is a low true signal at the sub miniature D connector on the rear panel. U306F drives the channel closed output signal.

The external trigger input is buffered by U304C and U304D.

Power Supplies

Unless otherwise noted, components in this discussion are located on the A1 circuit assembly (34970-66501). The schematics begin on page 208.

The instrument uses two types of power supplies: *floating supplies* and *earth referenced supplies*. The floating supply outputs are ± 18 Vdc, +5 Vdc, and a 6 Vrms center tapped filament supply for the vacuum fluorescent display. The earth referenced and backplane circuits are powered from a single +5 Vdc supply.

The ac mains are connected by module P1. This module includes the functions of mains connection and line voltage selection (100/120/220/240). The internal DMM automatically configures for the applied line frequency by counting the frequency of the output of clamp circuit CR106, R102, C103 (LSENSE).

The +5 volt floating supply is produced by bridge rectifier CR105, filter capacitor C104, and regulator U103. The output of CR105 is sensed by U104 and compared to the the voltage from battery BT101. U104 turns on the +5 V floating supply through Q120. If the output of CR105 falls below 6.8 V, U104 provides a PWRFAIL signal to the main processor. At initial power on, U104 resets the main processor with the FLT_RST line. This supply powers all floating logic. The internal DMM relay drive circuits are also powered from this supply.

The floating ± 18 volt supplies are produced by bridge rectifier CR109, filter capacitors C107 and C109, and regulators U105 and U106. These supplies are used to power all measuring circuits. In addition, the vacuum fluorescent display is driven from the ± 18 volt supplies.

A separate winding of T1 provides a center tapped 6 Vrms filament supply for the display. Q110A and Q110B turn on and off the filament supply in response to the FILPWR signal from the main controller through U107A .

The 5 volt earth referenced supply (+5V_ER) is produced by rectifier CR101, CR102, CR103, CR104, and regulator U101. This supply is earth referenced by the screw which mounts the PC board to the instrument chassis.

The unswitched +5V_ER supplies U305, U303, U320, and U302. The rear panel interfaces (HP-IB, RS-232, Alarms, and external triggers) are powered from the switched +5V_BP supply to ensure that when power is turned off no voltages are present at the interfaces.

The +5V_ER supply is switched by Q101A and Q101B to create the +5V_BP (backplane) and fan power supplies.

Undervoltage sensor U102 provides the earth reference controller reset at initial power on.

Front Panel

Unless otherwise noted, components in this discussion are located on the A2 circuit assembly (34970-66502). The schematics begin on page 213.

The front panel circuits consist of vacuum fluorescent display control, display high voltage drivers, and keyboard scanning. Communication between the front panel and floating logic circuits is accomplished through a 2-wire bi-directional serial interface. The front panel logic operates from -13 volts (logic 1) and -18 volts (logic 0). The two serial communication signals are level shifted by comparator U6 from the floating logic 0 V to 5 V levels to the -18 V to -13 V levels present on the front panel assembly. The front panel logic high supply (-13 volts) is produced from the -18 volt supply by voltage regulator U7.

Display anode and grid voltages are +18 volts for an on segment and -18 volts for an off segment. The -11 V cathode bias for the display is provided by the main pc boards filament winding center tap bias circuit A1CR108, A1R106, and A1C106 shown on the power supply schematic (see page 208).

Keyboard scanning is accomplished through a conventional scanned row-column key matrix. Keys are scanned by outputting data at microprocessor U1 port pins P0.0 through P0.4 to poll each key column for a key press. Column read-back data are read by the microprocessor at port pins P2.0 through P2.3 for decoding and communication to the floating logic circuits. Rotary knob quadrature inputs are read directly by the microprocessor port pins P2.6 and P2.7.

The standby power switch, S19, provides a low true signal to main controller A1U205. In turn, A1U205 takes actions that either place the instrument in the “standby mode” or “on” mode. In “standby”, both the filament supply to the front panel and the +5V_BP supply to the backplane, rear panel interfaces, and fan are turned off.

Backplane

Unless otherwise noted, components in this discussion are located on the A3 circuit assembly (34970-66503). The schematics begin on page 215.

The backplane contains three connectors, P101, P102, and P103 for connection to the plug-in modules. The parallel lines in these connectors are divided into two groups to form the analog bus and digital bus.

Analog Bus

The analog bus connects the signals from the plug-in modules to the Internal DMM. There are five lines in the analog bus, HI, LO, OHMS_HI, OHMS_LO, and AMPS. The HI and LO lines are protected from overvoltages by E101, E102, RV101, RV102, R101, R160, L101, L102, and C109.

P105 makes the analog bus connection to the internal DMM.

Digital Bus


The digital bus uses 10 lines for communication and control. P104 makes the digital bus connection to the earth referenced logic and floating logic.

Signal	P101, P102, P103 pins	Comments
Slot ID	A6, A7, A8	Unique binary code for each slot.
DATA_IN	B6	Serial module data from the floating logic.
DATA_OUT	C6	Serial module data to the floating logic.
DGND	A5, B5, B7, C5, C7	Earth referenced digital ground.
+5 V	A3, B3, C3	Earth referenced module power supply.
Earth Ground	A1, B1, C1	Earth referenced zap return ground.
RST	B8	Module reset from the earth referenced logic.
SRQ	C8	Module service request to the earth referenced logic.

Internal DMM

DMM Block Diagram

The internal DMM block diagram is shown on the system block diagram on page 205. A portion of the block diagram is shown below.

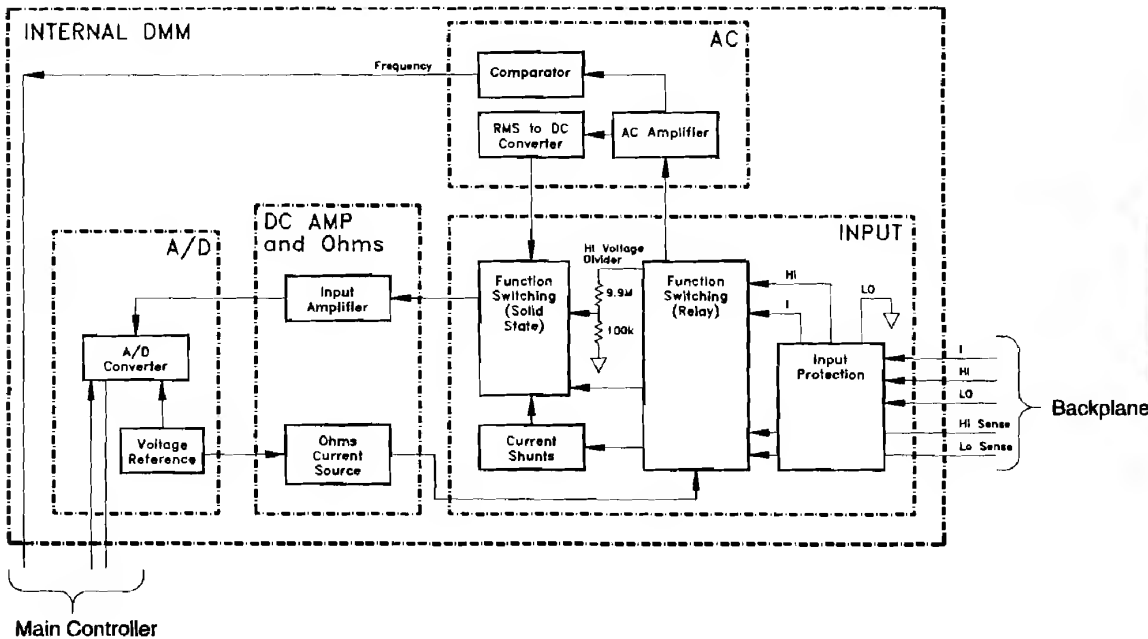

Input

Unless otherwise noted, components in this discussion are located on the A4 circuit assembly (34970-66504). The schematics begin on page 218.

The purpose of the Input section is to connect the **Input HI** terminal to the various measuring functions. This is accomplished through K102, K103, and K104. Additionally, connections are made for the 4-wire ohms **HI Sense** and **LO Sense** inputs. Shunt selection (ranging) and voltage sensing are also performed for the current function. The table below shows the state of each relay for each measuring function. All relay coils are driven from U150.

Function	K102	K103	K104	Sense at:
0.1 V – 10 Vdc	Set	Set	Set [1]	U101-5
100 V – 300 Vdc	Set	Reset	Set	U102-12
2-Wire Ohms	Reset	Set	Reset [2]	U101-5
4-Wire Ohms	Reset	Set	Reset [2]	[3]
AC Voltage	Set	Reset	Reset	AC_IN
Frequency/Period	Set	Reset	Reset	AC_IN
3 A, 1A DC I	Reset	Set	Reset	U101-10
100 mA, 10 mA DC I	Set	Set	Reset	U101-10
1A AC I	Reset	Set	Set	AC_IN

[1] K104 will be reset when input resistance is selected to >10,000 M Ω through the menu.

[2] K104 will be set for the 100 M Ω range.

[3] Configurations shown are for the current source output (HI) terminal. The measurement sense is accomplished through the Sense HI / Sense LO terminals.

Input Amplifier

Unless otherwise noted, components in this discussion are located on the A4 circuit assembly (34970-66504). The schematics begin on page 218.

The DC Amplifier circuit is used by every measuring function except frequency and period. Analog switch U101B selects various input signals for measurement by the ADC. Switch U101B has three sources which can be dynamically selected: *measure customer input* (MC), *measure zero input* (MZ), and *precharge* (PRE). The MC state is the actual input measurement. The MZ state measures internal offset voltages which are also present in the MC measurement. The final measurement result is computed from MC-MZ. The PRE state is used to “precharge” internal capacitances to reduce charge injection to the input terminal from the dynamic switching of MC and MZ. Autozero off disables the dynamic switching of the amplifier input. However, a new MZ value is automatically taken whenever a new function or range is selected, even if autozero is turned off.

In the dc voltage function, ranging is accomplished through both input relay switching (K102-K104) and solid state switching (U101). As a result, the input to the ADC has the same nominal 10 V value for a full scale input on each range. The dc input amplifier is comprised of source follower dual FET U104, amplifier U106, and associated bias circuitry. The feedback resistors U102C and switches U101C select non-inverting amplifier gains of x1, x10, and x100 for the dc input amplifier circuit. Amplifier output ADIN drives the dc input to the a-to-d converter for all measuring functions.

DCV Range	U102A Divider	U101 Input	Amplifier Gain	ADC Input
100 mV		Pin 5	x100	10 V
1 V		Pin 5	x10	10 V
10 V		Pin 5	x1	10 V
100 V	1/100	Pin 8	x10	10 V
1000 V	1/100	Pin 8	x1	10 V

In the DC current function, a current is applied between the **Input I** and **LO** terminals. Ranging is accomplished by relay K102 and amplifier gain switching in U101. Since a known resistor (the shunt resistor) is connected between these terminals, a voltage proportional to the unknown current is generated. The voltage sensed at R121 is measured by the multimeter's dc circuitry. The table below illustrates the dc current measuring function configurations.

DCI Range	Shunt Resistor	U101-10 Input	Amplifier Gain	ADC Input
1A	0.1 Ω	100 mV	x100	10V
100 mA	5.1 Ω	510 mV	x10	5.1V
10 mA	5.1 Ω	51 mV	x100	5.1V

Resistance measurements are made by applying a known current through an unknown resistance. The resulting voltage drop across the unknown resistance is then measured by the multimeter's dc circuitry. The 100 M Ω range is measured using the known internal 10 M Ω resistance (U102A) in parallel with the unknown input resistance while applying the 500 nA current source. The result is computed from the measured data. The internal 10 M Ω resistance is determined whenever a zero calibration is performed.

In the 2-wire ohms function, the voltage drop is measured across the **Input HI** and **Input LO** terminals. In the 4-wire ohms function, the voltage is measured across the **HI Sense** and **LO Sense** terminals. Lead resistances in series with the current source (**Input HI-LO**) are not part of the final measurement. However, they do reduce the available current source compliance voltage for the resistor under test. The ohms current source will become non-linear when the compliance voltage limit is exceeded. The full scale voltage developed across the unknown resistor and the dc amplifier gain for each resistance range are tabulated below.

Ohms Range	Voltage Across R	Amplifier Gain	ADC Input
100 Ω	100 mV	x100	10 V
1 k Ω to 100 k Ω	1 V	x10	10 V
1 M Ω	5 V	x1	5 V
10 M Ω	5 V	x1	5 V
100 M Ω	4.5 V	x1	4.5 V

Ohms Current Source

Unless otherwise noted, components in this discussion are located on the A4 circuit assembly (34970-66504). The schematics begin on page 218.

The ohms current source flows from the **Input HI** terminal to the **Input LO** terminal for both the 2-wire and 4-wire ohms functions. Each current value is generated by forcing a stable, precise voltage across a stable resistance. The value of the current becomes part of the range gain constant stored during calibration.

The +7 V reference voltage is used to generate a stable reference current with U201A. R201 and R202 are the resistance references for the current sources as shown in the table below. The IREF current is used to produce a precise voltage drop across the 28.57 k Ω resistor in U102D-4. The IREF generated using R202 produces an approximate 5 V drop across the 28.57 k Ω resistor. The IREF generated using R201 produces an approximate 0.5 V drop. This voltage is used to force a reference voltage across the selected current source range resistor (5 k Ω , 50 k Ω , 500 k Ω , 1 M Ω) by U201B. The resulting precision current flows through JFET Q202 and protection circuit Q203 to Q211, and CR202 to relay K102 where it is switched to the **Input HI** terminal for ohms measurements.

The protection circuits are designed to protect the ohms current source from inadvertently applied voltages in excess of ± 1000 V. Protection from large positive voltages is provided by the reverse breakdown voltage of CR202. Protection from large negative voltages is provided by the sum of the collector to base breakdown voltages of Q203, Q205, Q207, and Q209. Bias for these transistors is provided by Q211 and R203 to R206 while negative over voltages are applied.

Ohms Range	Current	Open Circuit Voltage	Compliance Limit	Reference	Isource R U102D
100 Ω	1 mA	9 V	2.5 V	R202	5 k Ω
1 k Ω	1 mA	9 V	2.5 V	R202	5 k Ω
10 k Ω	100 μ A	9 V	4 V	R202	50 k Ω
100 k Ω	10 μ A	9 V	4 V	R202	500 k Ω
1 M Ω	5 μ A	9 V	8 V	R202	1 M Ω
10 M Ω	500 nA	14 V	10 V	R201	1 M Ω
100 M Ω ^[1]	500 nA ^[1]	5 V		R201	1 M Ω

[1] Measured in parallel with the internal 10 M Ω resistor.

AC Circuit

Unless otherwise noted, components in this discussion are located on the A4 circuit assembly (34970-66504). The schematics begin on page 218.

The multimeter uses a true RMS ac-to-dc converter to measure ac voltages and currents. The ac-to-dc converter changes the input ac voltage to a dc voltage. All voltage ranging is performed in the ac circuit so that the input to the multimeter's dc circuitry (AC_OUT) is nominally 2 Vdc for a full scale ac input. The dc amplifier is always configured for x1 gain in ac functions (voltage, current, frequency, and period). Relay K104 connects the ac circuit to either the **Input HI** terminal or to R121, the current function voltage sense point. Note that the input to the ac circuit may contain a dc bias from the applied ac signal.

Input coupling capacitor C301 blocks the dc portion of the input signal. Only the ac component of the input signal is measured by the multimeter. The ac circuit voltage ranging comprises two gain stages U301 and U305/U312. The voltage gains for each stage are tabulated below.

Function	Range	Shunt Resistor	1st Stage	2nd Stage	ADC Input
ACV, Freq, or Period	100 mV		x0.2	x100	2 Vdc
	1 V		x0.2	x10	2 Vdc
	10 V		x0.2	x1	2 Vdc
	100 V		x0.002	x10	2 Vdc
	300 V		x0.002	x1	1.4 Vdc
ACI	10 mA	5.1 Ω	x0.2	x100	0.2 Vdc
	100 mA	0.1 Ω	x0.2	x100	1 Vdc
	1 A	0.1 Ω	x0.2	x100	2 Vdc

The 1st stage is a compensated attenuator implementing a gain of x0.2 or x0.002 as selected by U304A and U304B. Each voltage range has a unique 50 kHz frequency response correction produced by a programmable variable capacitor connected across R304.

The programmable capacitance is implemented by varying the signal level across a compensating capacitor. In the x0.2 configuration, low frequency gain is set by R301, R302, and R304. The variable gain element U302/U303 essentially varies the value of C306 from 0 to 1 times its value in 256 steps. The exact gain constant is determined during the 50 kHz ac voltage range calibration procedure. In the x0.002 configuration, low frequency gain is set by R301, R302, and R303. The variable gain element U302/U303 essentially varies the value of C305 plus C306 from 0 to 1 times their value in 256 steps. The exact gain constant is determined during the 50 kHz ac voltage range calibration procedure.

The second stage is made up of two amplifiers (U305 and U312) each configured for a fixed gain of x10. Overall 2nd stage gains of x1, x10, and x100 are produced by routing the 1st stage output either around, or through one or both amplifiers as shown in the table below.

2nd Stage Gain	U306A	U306B	U306C	U306D	U304C
x1	ON	OFF	OFF	OFF	OFF
x10	OFF	ON	OFF	ON	OFF
x100	OFF	OFF	ON	ON	ON

The output of the 2nd stage is connected to the rms-to-dc converter stage. Any residual dc offset from the amplifier stages is blocked by capacitor C316. Buffer U307 drives the input to the rms-to-dc converter as well as the frequency comparator (U310A) input. The rms-to-dc converter has two selectable averaging filters (C318 and C318 plus C321) for the analog computer circuit of U308. The two analog averaging filters together with digital filters running in the main CPU implement the three selectable ac filters: slow, medium, and fast. The faster analog filter (using C318) is used for all AC V, AC I, and frequency or period autoranging. The slower analog filter is used only with the slow and medium ac filter choices.

In frequency or period measurements, U310A generates a logic signal (FREQIN) for every input zero crossing. The ac sections FREQRNG dc output is measured directly by the main CPU's 10-bit ADC during frequency or period measurements. This lower resolution measurement is sufficient to perform voltage ranging decisions for these functions. The frequency comparator output is disabled during ac voltage and current measurements by U310B forcing U310A's input to -15 volts.

A-to-D Converter

Unless otherwise noted, components in this discussion are located on the A4 circuit assembly (34970-66504). The schematics begin on page 218.

The analog-to-digital converter (ADC) is used to change dc voltages into digital information (schematic shown on page 9-12). The circuitry consists of an integrator amplifier (U402 and U420), current steering switch U411, resistor network U102E, voltage reference U403, ADC controller U209, and residue ADC U205.

The ADC method used is called *multislope III*. It is based on patented Hewlett-Packard ADC technology. Multislope III is a charge balancing continuously integrating analog-to-digital converter. The ADC charge balancing algorithm is always running, even when the multimeter is not triggered. The input voltage continuously forces charge onto the integrator capacitors C400 and C401 through U102E–R16.

Switches U411A and U411B steer fixed positive or negative reference currents onto the integrator capacitor to cancel, or balance, the accumulated input charge. The level shifted (R403 and R406) output of the integrator is checked every 2.66 μ s by the A1U209 COMP input. Logic state machines in A1U209 control the U411 current steering to continuously seek an approximate 2.5 V level on the integrator amplifier output, FLASH. If the ADC input voltage ADIN is between ± 15 V, the integrator output (FLASH) will remain within the 0 V to 5 V range of the A1U205 on-chip ADC. An input greater than +15 V may cause the integrator output (U402–6) to saturate at about –18 V. An input less than –15 V may cause U402 to saturate with an output of about +18 V. The A1U205 ADC input (FLASH) is clamped to 0 V or 5 V by R405 and CR403 to protect A1U205.

The integrator amplifier is formed by U402 and U420. Resistors R420 and R421 affect the amplifier stability. Amplifier oscillation may occur if their values are incorrect. Amplifier U420 improves the offset voltage characteristics of integrator amplifier U402.

Each analog-to-digital conversion begins when the multimeter is triggered. The ADC starts by clearing the integrator slope count in A1U209. At the end of the integration period, the slope count is latched. The slope count provides the most significant bits of the input voltage conversion. The least significant bits are converted by the on-chip ADC of CPU A1U205.

The instrument precision voltage reference is U403. Resistor R409 provides a stable bias current for the reference zener diode. R408 and CR404 provide a bias to assure that the reference zener biases to +7 V during power up. IC U400A amplifies the voltage reference to +10 V while amplifier U401A inverts the +10 V reference to -10 V. The reference voltages force precision slope currents for the integrating ADC through U102E-R17, R18.


Switch Modules

In general, all the switch modules share a common module control circuitry. This circuitry is described below. Each module is described in further detail on the following pages.

Switch Module	Name	Page
HP 34901A	20 Channel MUX with T/C Compensation	124
HP 34902A	16 Channel Reed MUX with T/C Compensation	126
HP 34903A	20 Channel Actuator	128
HP 34904A	4 X 8 Matrix Switch	129
HP 34905A	50 Ω Dual 4:1 VHF MUX	130
HP 34906A	75 Ω Dual 4:1 VHF MUX	130
HP 34908A	40 Channel Single-Ended MUX with T/C Compensation	131

Switch Module Control

A simplified block diagram of a typical module controller is shown below.

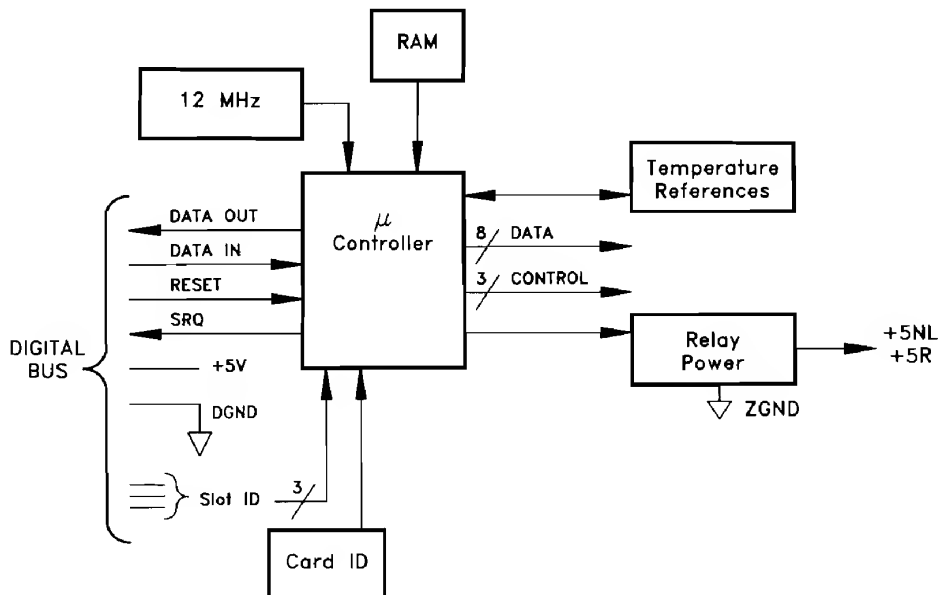

In addition to the +5 Volt power supply (Vcc) and ground, the module controller uses four lines for control and communication:

- RESET, from the Earth Referenced Logic A1U305. RESET is common to all three slots. The module controller performs a reset when this line goes high. Reset conditions vary for each plug-in.
- SRQ, to the Earth Referenced Logic A1U305. The SRQ line is a wired-OR line that can be driven by any plug-in. Consequently, any module that asserts SRQ (line low), asserts this line in all other slots and at the Earth Reference Logic.
- DATA IN, from the Floating Logic A1U205 via the opto isolator A1U312. This line is connected in common to all three slots.
- DATA OUT, from the module controller to the Floating Logic A1U205 via the opto isolator A1U213. This line is a wired-OR line that can be driven by any module.

The DATA IN and DATA OUT lines are optically isolated from the floating logic controller. These lines communicate with the Floating Logic using an asynchronous serial bit stream.

The serial communications use an 11 bit protocol; a start bit, 8 data bits, an attention bit, and a stop bit. The attention bit is 1 if the 8 data bits are an address/command, or 0 if the 8 data bits modify or provide data for the previously sent command.

The module controller uses the hardwired slot-ID bits to decode the serial bit stream address. When the address/command message address matches the slot-ID, the plug-in is selected and responds to the following commands. All other plug-ins will ignore the commands until a new address/command message is received.

A 12 MHz crystal, Y101 is the clock for the module controller. The module ID is a four bit pattern set through R106, R107, R108, and R109. The Ferro-electric RAM U150 provides data storage of the relay usage on the module (*see page 55*) and the thermocouple reference junction temperature corrections (*see page 94*). Data in and out of U150 is serial.

The HP 34901A, HP 34902A, and HP 34908A each have two onboard, solid state temperature sensors, U151 and U152, physically located near the isothermal block at the input connections. The temperature sensors are used as the thermocouple temperature reference.


U101 controls the relays on the module using an 8-bit data bus and 3 control lines. The data lines are latched and applied to the relay drivers.

U101 enters a low-power idle mode when inactive. U101 responds when a command is received or when a scheduled reference junction temperature measurement is taken.

The relays use a buffered +5 Volt power supply. U101 supplies two drive enable lines (DR_EN and +5NL_EN) that connect Vcc from the digital bus with the relay drive lines through Q101 (+5R or +5NL). To minimize the current through DGND caused by static discharge, the ground return (ZGND) is isolated from the backplane ground through a bead L102.

Relay Drivers

Two types of single-coil relays are used on the switch modules: latching and non-latching. Typical driver configurations are shown below.

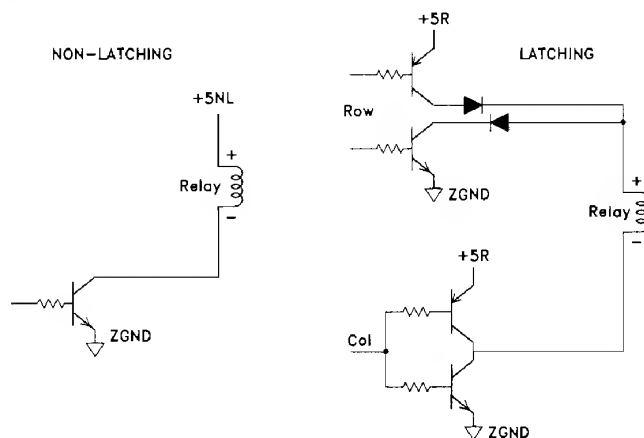

The non-latching relay contacts are in the set position (closed) when current flows through the coil. When the current is removed, the relay resets (opens). The positive side of the relay coil is connected to +5NL. The negative side of the relay coil is connected to ZGND through a single NPN transistor. The transistor and +5NL must be on for the relay to stay in the set position.

The polarity of the current flow through the latching relay coil determines the set (closed) or reset (open) position of the relay contacts. Latching relays are driven by row and column latches or complimentary transistor pairs.

To set a relay (close a channel) in the row column driver circuitry, the appropriate row driver PNP transistor is turned on connecting the +5R supply to the positive side of several relay coils and ZGND is applied to the negative side of the desired relay coil through a column driver NPN transistor. To reset a relay, ZGND is applied through an NPN row driver transistor and +5R through a PNP column driver.

Tree latching relays are driven by complimentary transistor pairs that steer the current through the relay coil.


The +5R supply is only enabled while the relay changes state. The table below shows the times required for the relays to change state.

Switch Module	Open	Close
HP 34901A	6 ms	6 ms
HP 34902A	0.40 ms	1.25 ms
HP 34903A	6 ms	6 ms
HP 34904A	6 ms	6 ms
HP 34905A/06A	10 ms	15 ms
HP 34908A	6 ms	6 ms

HP 34901A

Components in this discussion are located on the A1 circuit assembly (34901-66501). The schematics begin on page 223.


The control circuitry has four groupings of latches, relay drivers and relays. The three control lines (SEL_A, SEL_B, and SEL_C) from the module controller are divided into five control lines by the binary to octal converter U109.

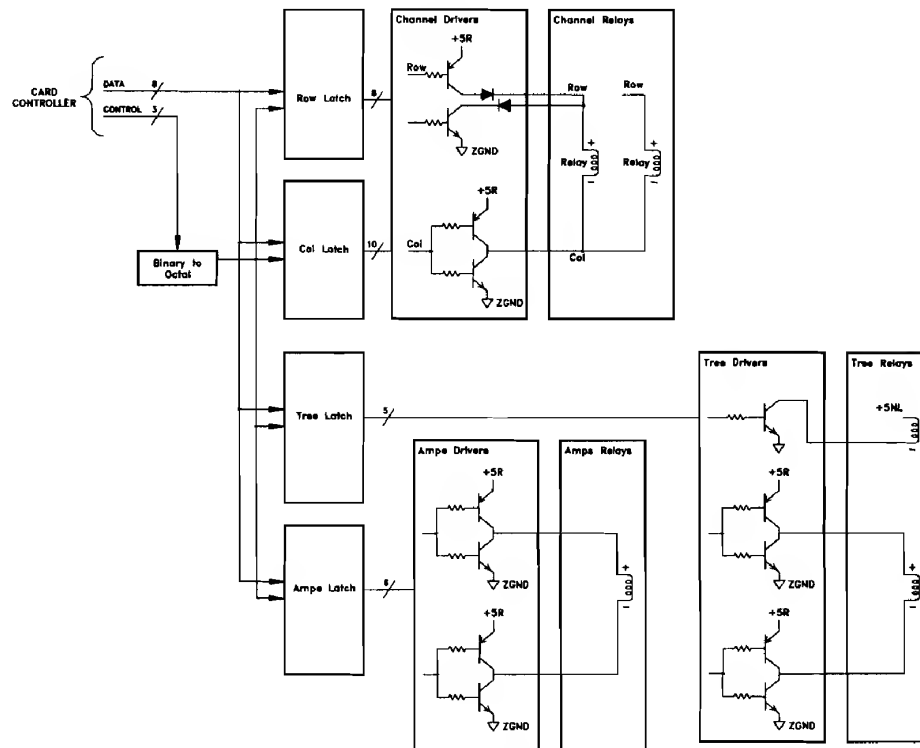

The row latch, U102, and column latches, U103 and U104, control the relays. The row drivers are divided into four groups of set and reset drivers. Each group of row drivers controls five relays. The column drivers operate as a pair. There are ten column drivers each controlling two relays.

The analog bus backplane relays are non-latching.

The 20 channels are divided into two banks. The banks are combined by closing K422 for voltage and 2-wire Ohms switching. When K422 is open, the banks are electrically independent of each other and this configuration is used for 4-wire Ohms multiplexing where the Ohms current sources are connected to channels 1 through 10 and the sense is obtained from channels 11 through 20. K421 and K423 control the connection to the analog bus for measurements using the Internal DMM.

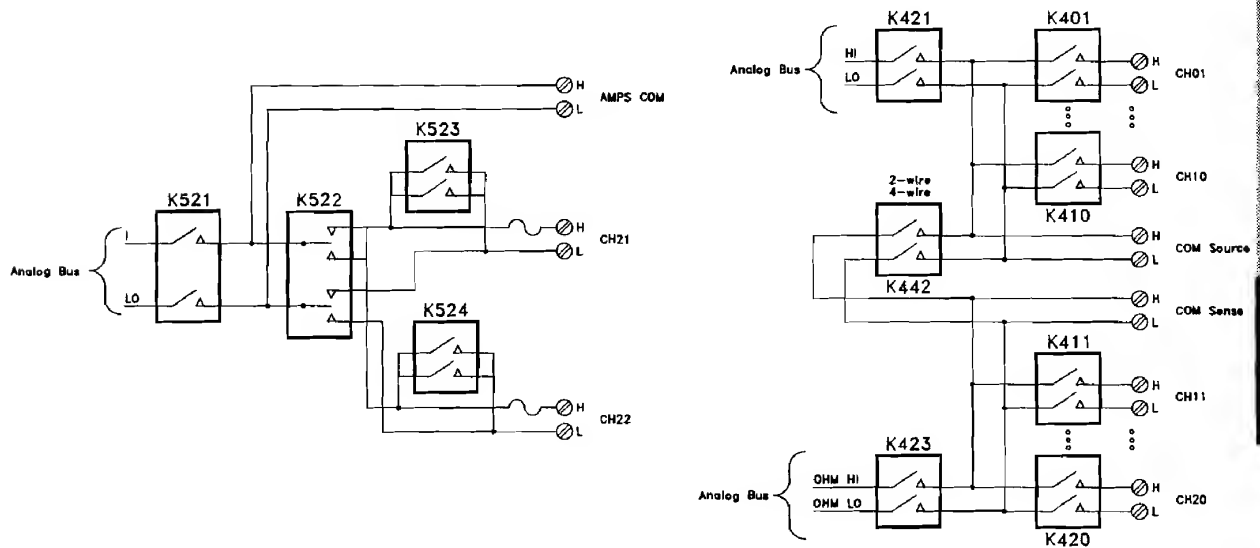


The current measurement channels are selected by relay K522. Relays K523 and K524 short the inputs when a channel is not selected. Relay K521 makes the connection to the analog bus for measurement by the Internal DMM.

HP 34902A


Components in this discussion are located on the A1 circuit assembly (34902-66501). The schematics begin on page 229.

The control circuitry has of two groupings of latches, relay drivers and relays. The 16 voltage and resistance measurement channels are directly driven. Tree switching controls the 2-wire/4-wire Ohms operation and connections to the analog bus.

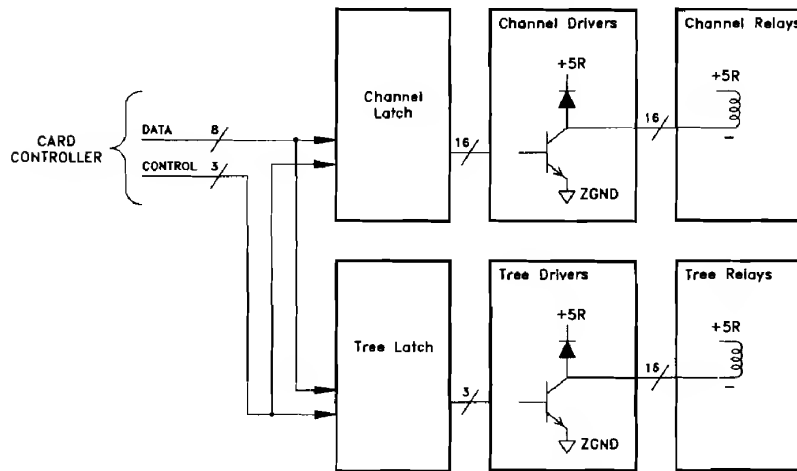

The reed relays are non-latching and the relay driver and +5R is applied while a channel is closed.


The 16 channels are divided into two banks. The banks are combined by closing K327 for voltage and 2-wire Ohms switching. When K327 is open, the banks are electrically independent of each other and this configuration is used for 4-wire Ohms multiplexing where the Ohms current source is connected to channels 1 through 8 and the sense is obtained from channels 9 through 16. Relays K326 and K328 control the connection to the analog bus for measurements using the internal DMM.

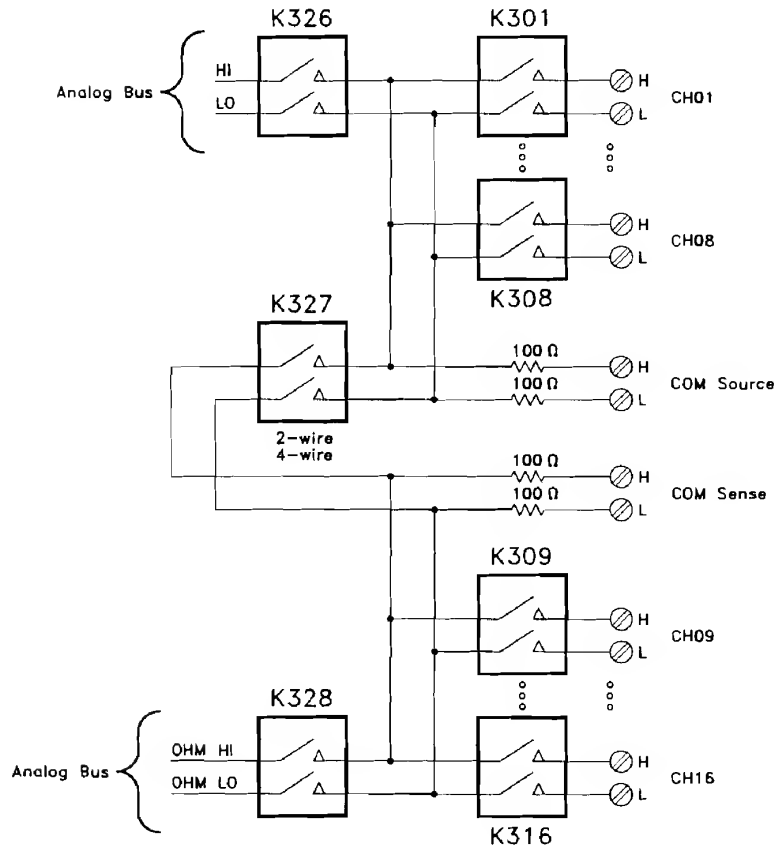

HP 34903A


Components in this discussion are located on the A1 circuit assembly (34903-66501). The schematics begin on page 234.

The control circuitry has two grouping of latches, relay drivers and relays. The 20 channels are, for control purposes, arranged into 8 rows by 10 columns.

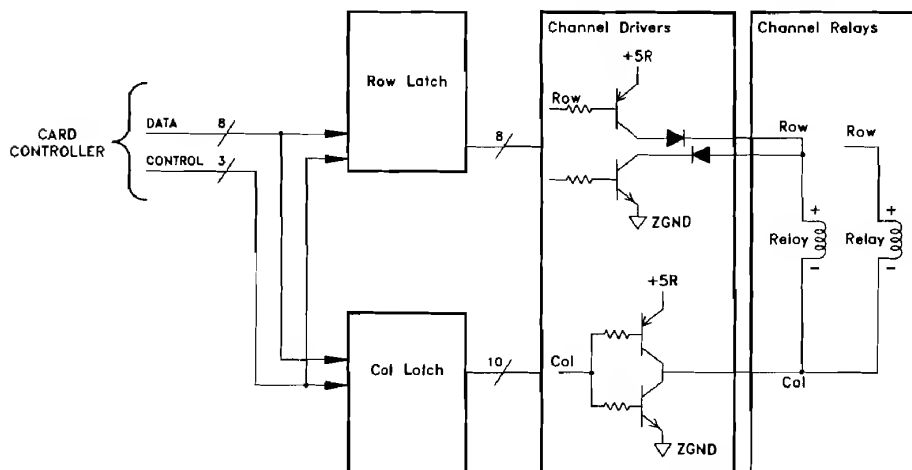

The row latch, U102, and column latches, U103 and U104, control the relays. The row drivers are divided into four groups of set and reset drivers. Each group of row drivers controls five relays. The column drivers operate as a pair. There are ten column drivers each controlling two relays.


The HP 34903A provides 20 channels of Form C switching.

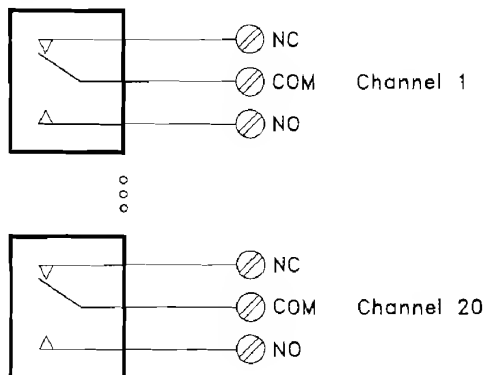

HP 34904A


Components in this discussion are located on the A1 circuit assembly (34904-66501). The schematics begin on page 238.

The control circuitry has four groupings of latches, relay drivers and relays divided into 4 rows by 8 columns.

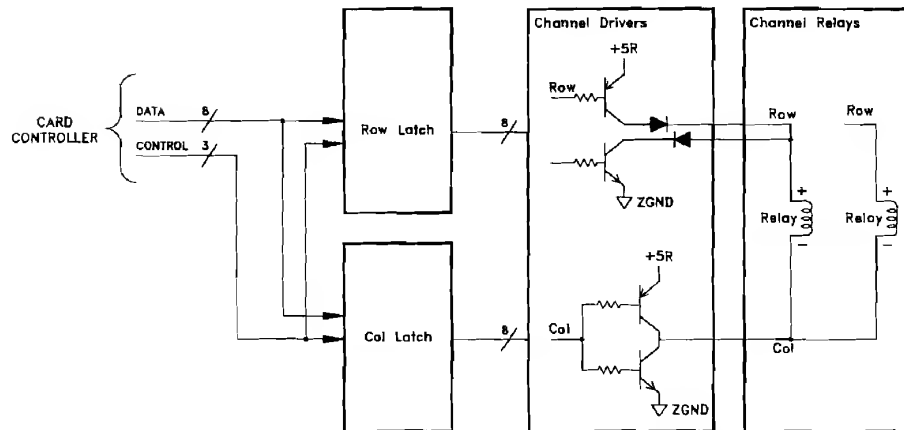

The row latch, U102, and column latch U103, control the relays. The row drivers are divided into four groups of set and reset drivers. Each group of row drivers controls eight relays. The column drivers operate as a pair. There are eight column drivers each controlling four relays.


The relays are arranged in 4 rows by 8 columns.

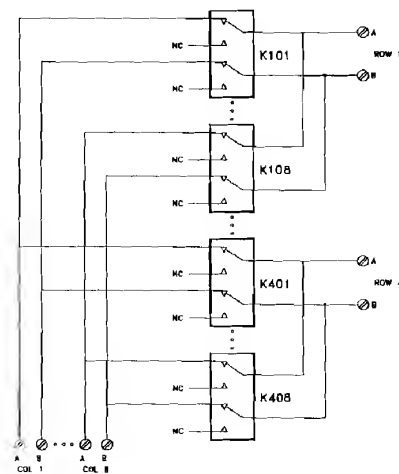

HP 34905A/34906A


Components in this discussion are located on the A1 circuit assembly (34905-66501 or 34906-66501). The schematics begin on page 242.

The control circuitry has of two grouping of buffers, relay drivers and relays, one for each multiplexer bank.

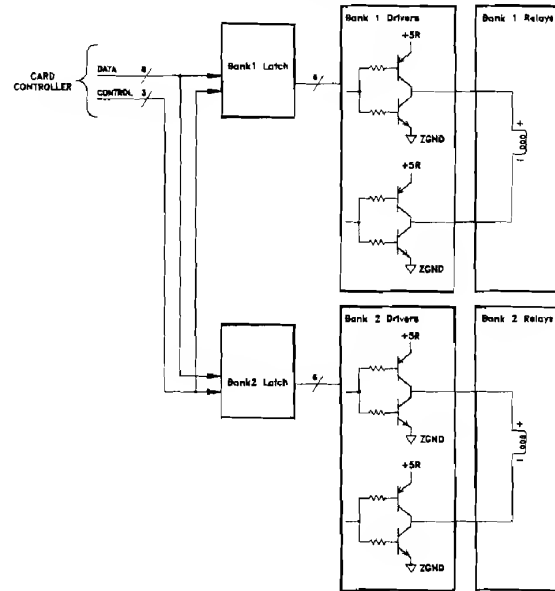

Bank1 latch, U102, and Bank2 latch, U103, control the relays. The bank drivers are divided into six groups of set and reset drivers. Each set and reset driver controls one relay. The column drivers operate as a pair. There are six column drivers each controlling a relay.


The relays are arranged into two independent banks:

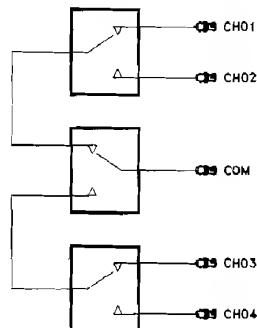

HP 34908A

Components in this discussion are located on the A1 circuit assembly (34908-66501). The schematics begin on page 251.


The control circuitry has three grouping of latches, relay drivers and relays. The 40 voltage and resistance measurement channels are, for control purposes, arranged into 8 rows by 10 columns. Tree switching controls bank selection and connections to the analog bus.

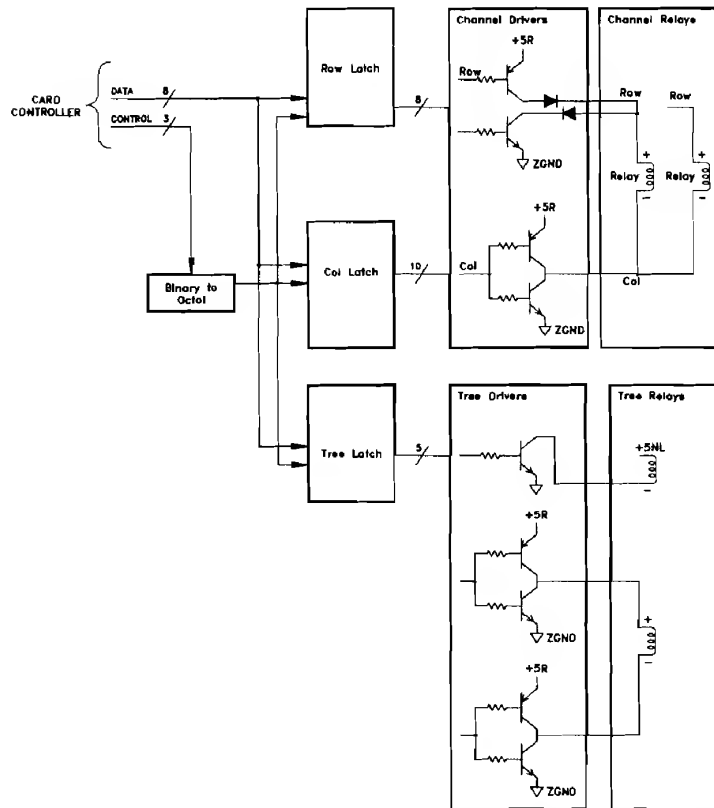

The row latch, U102, and column latches, U103 and U104, control the relays. The row drivers are divided into four groups of set and reset drivers. Each group of row drivers controls five relays. The column drivers operate as a pair. There are ten column drivers each controlling two relays.

The analog bus backplane relays are non-latching.

A single relay is used to switch two input channels. The choice of which channel is connected to the common is performed by relay K422. Channels are paired 20 channels apart (Ch 1 with Ch 21, Ch 2 with Ch 22, etc.) Relay K421 connects the common to the backplane analog bus for use with the internal DMM.

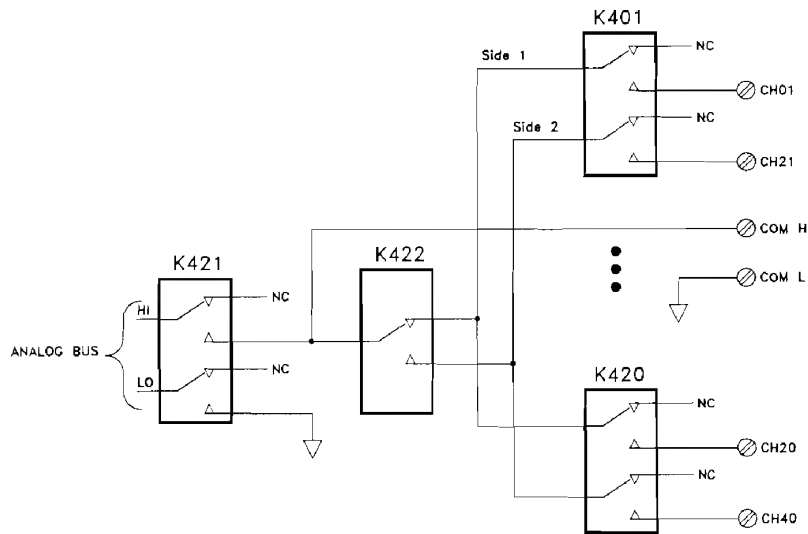


Multifunction Module

The HP 34907A Multifunction module contains two 8-bit digital input/output ports, a totalizer input, and two 16-bit analog outputs.

Multifunction Control

Components in this discussion are located on the A1 circuit assembly (34907-66501). The schematics begin on page 245.

A simplified block of the module control circuit is shown below.

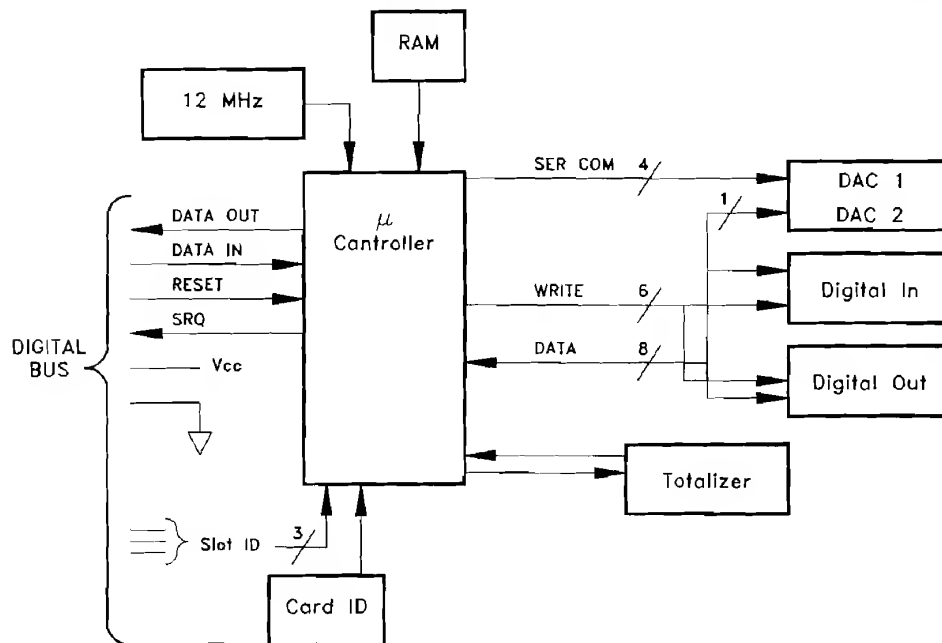

In addition to the +5 Volt power supply (Vcc) and ground, the module controller uses four lines for control and communication:

- RESET, from the Earth Referenced Logic A1U305. RESET is common to all three slots. The module controller performs a reset when this line goes high. Reset conditions vary for each plug-in.
- SRQ, to the Earth Referenced Logic A1U305. The SRQ line is a wired-OR line that can be driven by any plug-in. Consequently, any module that asserts SRQ (line low), asserts this line in all other slots and at the Earth Reference Logic.
- DATA IN, from the Floating Logic A1U205 via the opto isolator A1U312. This line is connected in common to all three slots.
- DATA OUT, from the module controller to the Floating Logic A1U205 via the opto isolator A1U213. This line is a wired-OR line that can be driven by any module.

The DATA IN and DATA OUT lines are optically isolated from the floating logic controller. These lines communicate with the Floating Logic using an asynchronous serial bit stream.

The serial communications use an 11 bit protocol; a start bit, 8 data bits, an attention bit, and a stop bit. The attention bit is 1 if the 8 data bits are an address/command, or 0 if the 8 data bits modify or provide data for the previously sent command.

The module controller uses the hardwired slot-ID bits to decode the serial bit stream address. When the address/command message address matches the slot-ID, the plug-in is selected and responds to the following commands. All other plug-ins will ignore the commands until a new address/command message is received.

A 12 MHz crystal, Y101 is the clock for the module controller. The module ID is a four bit pattern set through RP102. The Ferro-electric RAM U102 provides data storage of the calibration constants for the analog output channels. Data in and out of U102 is serial.


8 data lines, connected to U101 port 1, are used by the digital input and output ports. One of the data lines is used to send serial data to the analog output channels. The totalizer edge count is controlled by U101 P0.6 and read at U101 P3.4.

U101 enters a low-power idle mode when inactive. U101 responds when a command is received or when a scheduled alarm scan is needed.

Totalizer

Components in this discussion are located on the A1 circuit assembly (34907-66501). The schematics begin on page 245.

A simplified block diagram of the totalizer input is shown below.

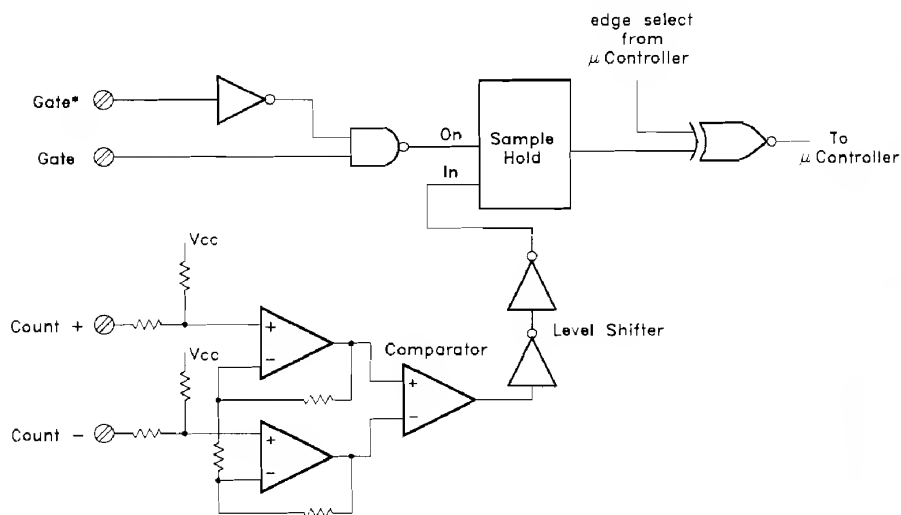

The totalizer counts signals connected to the COUNT+ and COUNT- inputs. Two op-amps, U108A and U108B, are used for input signal conditioning. Comparator U109 determines the signal trigger levels based upon the setting of the jumper at P102. With the P102 jumper in the TTL position, the totalizer counts pulses with TTL trigger levels. With the jumper at P102 in the AC position the trigger level is at zero.


The GATE and GATE* input signals control when counting occurs. If no signal is connected, the totalizer counts any changing signal on the inputs. A TTL low on the GATE input or a TTL high on GATE* input will halt counting.

Count edge selection is controlled from a U101 port bit (P0.6) through the exclusive OR gate U111. When the P0.6 signal is low, the count increments on the rising edge of the input signal. When the P0.6 signal is high, the count increments on the falling edge of the input signal.

Analog Output

Components in this discussion are located on the A1 circuit assembly (34907-66501). The schematics begin on page 245.

A simplified block diagram of the analog output channels is shown below.

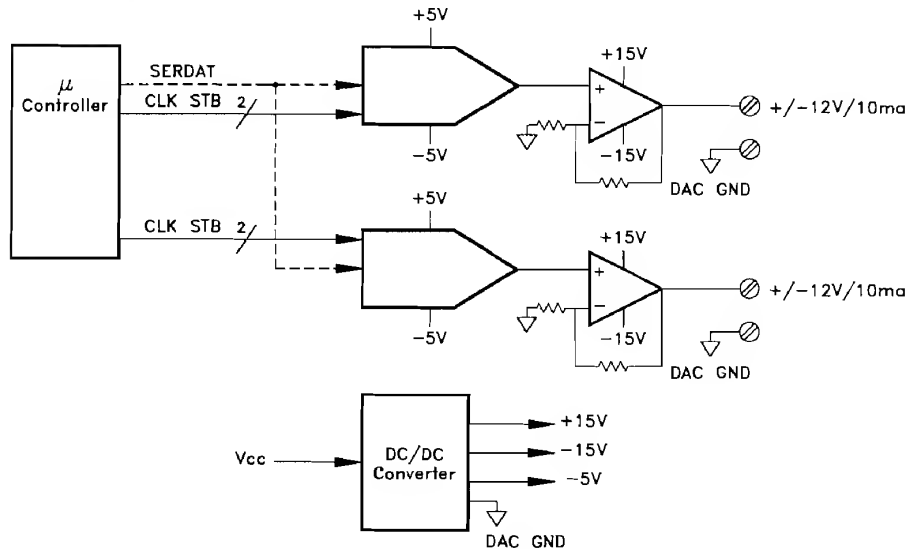

Communication with each DAC (U503 and U504) is via three lines: SERSTB, DACCLK, and SERDAT. Each DAC has a voltage output of ± 3 V. U505 and U506 amplify this voltage to the $\pm 12V$ output.

A DC/DC converter is used to provide the $\pm 15V$ supplies to U505 and U506. The $\pm 15V$ supplies also are used at the input of the totalizer. U502 provides the -5 V supply used by the DACs.

A line from U101 P0.4 is used to control the output of U510. After a reset or power-up, U510 is held in the shutdown state. U101 turns on the DC/DC converter in response to commands from the main controller. The main controller paces the turn on of the DC/DC converters to ensure that if multiple modules are installed, the backplane power supply is not pulled down by the in-rush current of the DC/DC converters.

The 74HC240's, U205 and U206, provide the output high drive current necessary to maintain a TTL high output level (≥ 2.4 Vdc) under load.

At instrument turn-on, following a reset, and whenever the data lines are being read, the MOSFETs are in the passive high state, and the high output drivers are disabled. The resistor connected between the MOSFET's gate and ZGND holds the gate near ground potential when the module is initially turned-on to ensure that the MOSFET is in the passive high state.

The comparators U301, U302, U401 and U402 maintain correct TTL high and low levels by shifting the voltages from the input to compensate for the forward voltage drop of the blocking diode. A reference voltage of +2.1 Vdc (TTL_REF) is applied to the inverting input of the comparator. When the input voltage is in the range of 0 Vdc to +4.3 Vdc the blocking diode is forward biased and its forward voltage drop is added to the applied voltage. For example, when 0 Vdc is applied to the data line, +0.7 Vdc is present on the non-inverting input of the comparator and the comparator output is low. When the input signal level is above 1.4 Vdc, a voltage greater than +2.1 Vdc is applied to the non-inverting input of the comparator causing its output to go high. When the input signal is less than 1.4 Vdc, a voltage less than 2.1 Vdc is applied to the comparator's non-inverting input causing its output to go low. This ensures an input voltage < 1.4 Vdc is interpreted as a TTL low level and an input > 1.4 Vdc is interpreted as a TTL high level.

The pull-up resistor (connected to the comparator's non-inverting input) allows external ground connections and open circuits to be detected. When the data line is grounded, the blocking diode is forward biased applying a +0.7 Vdc level to the comparator, a TTL low. When the data line is allowed to float, the non-inverting input of the comparator pulls up to +5 Vdc, a TTL high.

The blocking diode on the output is used for circuit protection. The diode reverse biases when the applied voltage exceeds +4.3 Vdc preventing externally supplied current from being injected into the module's +5V supply line.

The MOSFETs have a built in zener diode that conducts at any voltage of ≈ 75 Vdc or greater. The zener diode provides protection from external over voltage situations including static electricity.

Service

Service

This chapter discusses the procedures involved for returning a failed instrument to Hewlett-Packard for service or repair. Subjects covered include the following:

- Operating Checklist, *on page 141*
- Types of Service Available, *on page 142*
- Repackaging for Shipment, *on page 143*
- Electrostatic Discharge (ESD) Precautions, *on page 144*
- Surface Mount Repair, *on page 144*
- To Replace the Power-Line Fuse, *on page 144*
(also depicted on page 42)
- Troubleshooting Hints, *on page 145*
- Self-Test Procedures, *on page 149*
- Battery Check and Replacement, *on page 154*
- Disassembly, *on page 156*

Operating Checklist

Before returning your instrument to Hewlett-Packard for service or repair check the following items:

Is the instrument inoperative?

- Verify that the ac power cord is connected to the instrument.
- Verify that the front-panel On/Standby switch has been pushed.
- Verify that the power-line fuse is installed and not open
(see page 42):

Use a 500 mA, 250V fuse for all power line settings.

- Verify the power-line voltage setting.
See "If the Instrument Does Not Turn On" on page 42.

Does the instrument fail self-test?

- Verify that the correct power-line voltage is selected.
See "If the Instrument Does Not Turn On" on page 42.
- Remove all input connections to the instrument.

Errors may be induced by ac signals present on the input wiring during a self-test. Long test leads can act as an antenna causing pick-up of ac signals.

Is the Current Measurement Function Inoperative?

- Verify the input protection fuses on the HP 34901A Multiplexer Module. Replace with a 1.5 A 250 V NTD fuse.

Note: the Current input is only available on channels 21 and 22 of the HP 34901A.

Types of Service Available

If your instrument or a plug-in module fails within three years of original purchase, Hewlett-Packard will repair or replace it free of charge. If your instrument or plug-in module fails after your three year warranty expires, HP will repair or replace it at a very competitive price. HP will make the decision locally whether to repair or replace your unit.

Standard Repair Service (worldwide)

Contact your nearest HP Service Center. They will arrange to have your instrument repaired or replaced.

Express Exchange (U.S.A. only)

You can receive a replacement instrument via overnight shipment for low downtime.

Note: *Express Exchange applies to the HP 34970A. Plug-in modules are not supported as exchange assemblies.*

- 1 Call 1-800-258-5165 and ask for "Express Exchange."
- You will be asked for your shipping address and a credit card number to guarantee return of your failed instrument.
- When exchanging the HP 34970A, *do not* ship plug-in modules with your instrument. Remove all plug-in modules and customer wiring before shipping to HP.
- If you do not return your failed instrument within 45 days, your credit card will be billed for a new unit.
- If you choose not to supply a credit card number, you will be asked to send your failed instrument to a designated HP Service Center. After the failed unit is received, HP will send your replacement instrument.

Express Exchange (continued)

- 2 HP will immediately send a replacement instrument to you via overnight shipment.
 - The replacement instrument will have a different serial number than your failed instrument.
 - If you can not accept a new serial number for the replacement instrument, use the Standard Repair Service option described above.
 - If your failed instrument was “in-warranty,” your replacement instrument continues the original three year warranty period. You *will not* be billed for the replacement instrument as long as the failed instrument is received by HP.
 - If your three year warranty has expired, HP will bill you for the exchange price — less than a new unit price. HP warrants exchange instruments against defects for 90 days or the remainder of your original warranty.

Repackaging for Shipment

For the *Express Exchange Service* described on the previous page, return your failed unit to the designated HP Service Center using the shipping carton of the exchange unit. A shipping label will be supplied. HP will notify you when your failed unit has been received.

If the unit is to be shipped to HP for service or repair, be sure to:

- Attach a tag to the unit identifying the owner and indicating the required service or repair. Include the model number and full serial number.
- Place the unit in its original container with appropriate packaging material.
- Secure the container with strong tape or metal bands.

If the original shipping container is not available, place your unit in a container which will ensure at least 4 inches of compressible packaging material around all sides for the instrument. Use static-free packaging materials to avoid additional damage to your unit.

HP suggests that you always insure shipments.

Electrostatic Discharge (ESD) Precautions

Almost all electrical components can be damaged by electrostatic discharge (ESD) during handling. Component damage can occur at electrostatic discharge voltages as low as 50 volts.

The following guidelines will help prevent ESD damage when servicing the instrument or any electronic device.

- Disassemble instruments *only* in a static-free work area.
- Use a conductive work area to dissipate static charge.
- Use a conductive wrist strap to dissipate static charge accumulation.
- Minimize handling.
- Keep replacement parts in original static-free packaging.
- Remove all plastic, foam, vinyl, paper, and other static-generating materials from the immediate work area.
- Use *only* anti-static solder suckers.

Surface Mount Repair

Surface mount components should *only* be removed using soldering irons or desoldering stations *expressly* designed for surface mount components. *Use of conventional solder removal equipment will almost always result in permanent damage to the printed circuit board and will void your Hewlett-Packard factory warranty.*

To Replace the Power-Line Fuse

The power-line fuse is located on the rear panel of the instrument, near the power line connector. A procedure to replace the fuse is given on page 42. Use a 500 mAT 250 V fuse for all power line settings.

Troubleshooting Hints

This section provides a brief check list of common failures. Before troubleshooting or repairing the instrument, make sure the failure is in the instrument rather than any external connections. Also make sure that the instrument is accurately calibrated within the last year (*see page 63*). The instrument's circuits allow troubleshooting and repair with basic equipment such as a 6½-digit multimeter.

Unit is inoperative

- Verify that the ac power cord is connected to the instrument.
- Verify that On/Standby switch has been pushed.
- Verify the power-line fuse is not open (*refer to page 42*):

Use a 500 mAT, 250V fuse for all power line settings.

- Verify the power-line voltage setting.
See "If the Instrument Does Not Turn On" on page 42.
- Remove all plug-in modules to verify that a plug-in module is not causing the failure.

Unit reports error 705

This error may be produced if you accidentally turn off power to the unit during a calibration or while changing a non-volatile state of the instrument. Recalibration or resetting the state should clear the error.

If the error persists, a hardware failure may have occurred.

Isolating to an Assembly

- Remove all plug-in modules to isolate between the instrument and the plug-in modules.
- Listen for a beep when you press the On/Standby switch. The main controller can operate the beeper even with a display failure.
- Listen for the fan when you press the On/Standby switch. Fan operation indicates some operation of the main controller and power supplies.
- Try to operate the instrument from a remote interface. If remote operations are normal, the display should be replaced or repaired.
- Isolate the internal DMM by removing it. The instrument should operate and pass self-test without the internal DMM installed. Disassembly procedures start on page 156.

Unit fails self-test

- Verify that the correct power-line voltage setting is selected.
- Remove all plug-in modules and run self-test again. If the instrument does not show a failure, replace or troubleshoot the plug-in module.
- To isolate the internal DMM, disassemble the instrument and remove the internal DMM. Disassembly procedures start on page 156. Run self-test again. If the self-test passes, troubleshoot or replace the Internal DMM. If the self-test fails, troubleshoot or replace the HP 34970A.

Power supplies


Verify the power supplies generated on the 34970-66501 circuit board.

The front panel filament voltage, + 5 V backplane and +5 V fan are switched by the On/Standby switch. All other power supplies operate whenever the AC power cord is connected.

Warning

- **Exposed Mains**
- **Do Not Touch**

To check the power supplies, remove the instrument cover as shown on page 156. The power supplies can be checked from the bottom of the instrument as shown below. Be sure to use the correct ground point when checking the supplies.

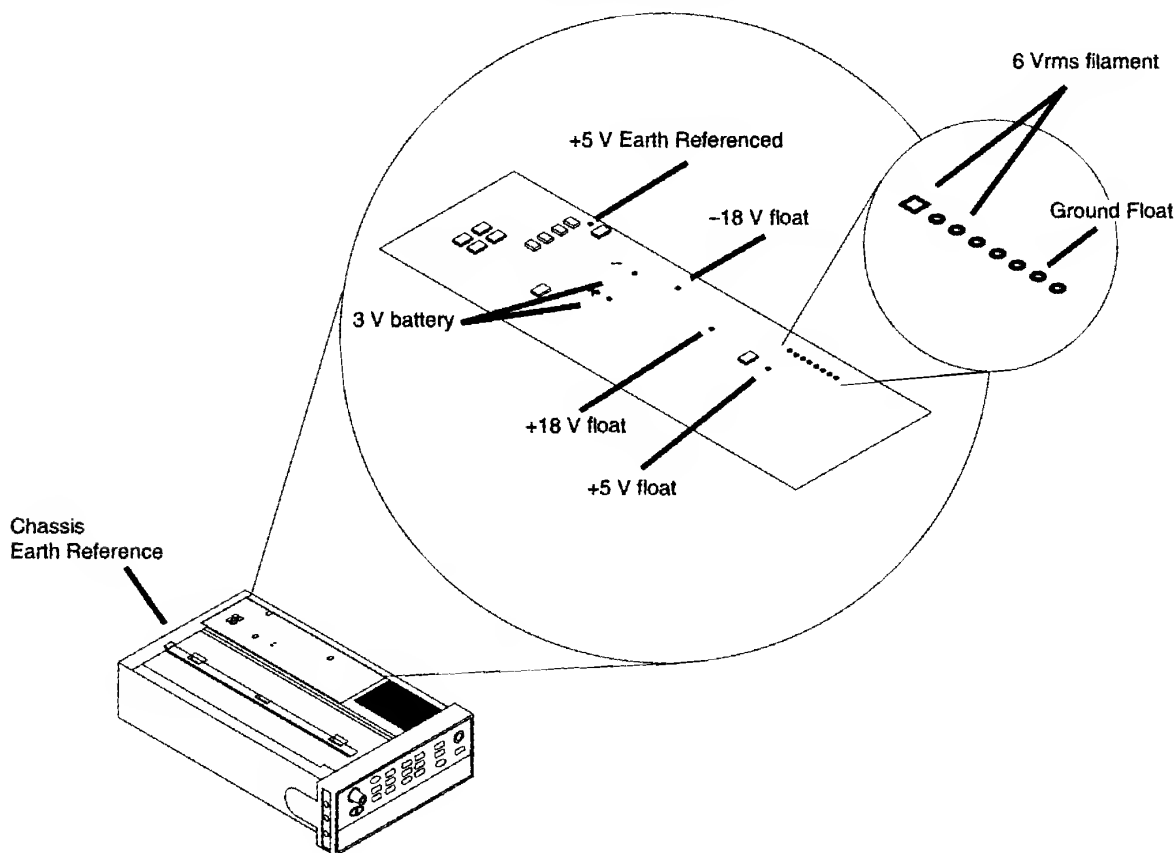

Continued on the next page ...

Power Supplies (continued)

The A1 power supplies are tabulated below.

Power Supply	Minimum	Maximum	Switched
+5 Earth Ref.	4.75 V	5.25 V	No
+5 Backplane and Fan	4.75 V	5.25 V	Yes
+5 Floating	4.75 V	5.25 V	No
+18 Floating	17.6 V	19.9 V	No
-18 Floating	-19.0 V	-16.8 V	No
6 Vrms Filament			Yes

- Check that the input to the supply voltage regulator is at least 1 V greater than its output.
- Circuit failures can cause heavy supply loads which may pull down the regulator output voltage.
- Always check that the power supplies are free of ac oscillations using an oscilloscope.
- All plug-in modules use the +5 V backplane supply. Some plug-in modules generate their own local power supplies.

Self-Test Procedures

Power-On Self-Test

Each time the instrument is powered on, a small set of self-tests are performed. These tests check that the minimum set of logic and measurement hardware are functioning properly. Any plug-in modules installed are verified for two-way communication with the main controller.

Complete Self-Test

Hold down any front panel key for 5 seconds while turning on the power to perform a complete self-test. The instrument beeps when the test starts. If all self-tests pass the display shows PASS for 5 seconds and the instrument returns to the last measurement function.

Plug-in Module Self-Test

No user self-test exists for the plug-in modules. The plug-in modules perform their own self-test when power is applied. Additionally, the mainframe checks two-way communication with all plug-in modules at power on.

Each plug-in module also performs error checking at regular intervals during operation and any errors detected are reported via the status system to the main controller.

Self-Tests

A complete self-test performs the following tests. A failing test is indicated by the test number and description in the display.

- 601 Front panel not responding** The main CPU A1U205 attempts to establish serial communications with the front panel processor A2U1. During this test, A2U1 turns on all display segments. Communication must function in both directions for this test to pass. If this error is detected during power-up self-test, the instrument will beep. This error is only readable from the remote interface.
- 602 RAM read/write failed** This test writes and reads a 55_h and AA_h checkerboard pattern to each address of RAM. Any incorrect readback will cause a test failure. This error is only readable from the remote interface.
- 603 A / D sync stuck** The main CPU issues an A / D sync pulse to A1U209 and A1U205 to latch the value in the ADC slope counters. A failure is detected when a sync interrupt is not recognized and a subsequent time-out occurs.
- 604 A / D slope convergence failed** The input amplifier is configured to the measure zero (MZ) state in the 10 V range. This test checks whether the ADC integrator produces nominally the same number of positive and negative slope decisions ($\pm 10\%$) during a 20 ms interval.
- 605 Cannot calibrate rundown gain** This test checks the nominal gain between the integrating ADC and the A1U205 on-chip ADC. This error is reported if the procedure can not run to completion due to a hardware failure.
- 606 Rundown gain out of range** This test checks the nominal gain between the integrating ADC and the A1U205 on-chip ADC. The nominal gain is check to $\pm 10\%$ tolerance.
- 607 Rundown too noisy** This test checks the gain repeatability between the integrating ADC and the A1U205 on-chip ADC. The gain test (606) is performed eight times. Gain noise must be less than ± 64 lsb's of the A1U205 on-chip ADC.

- 608 Serial configuration readback failed** This test re-sends the last 9 byte serial configuration data to all the serial path. The data is then clocked back into A1U209 and compared against the original 9 bytes sent. A failure occurs if the data do not match.
- 609 DC gain x1 failed** This test configures for the 10 V range. The dc amplifier gain is set to X1. The measure customer (MC) input is connected to the internal TSENSE source which produces 0.6 volts. A 20 ms ADC measurement is performed and checked against a limit of $0.6\text{ V} \pm 0.3\text{ V}$.
- 610 DC gain x10 failed** This test configures for the 1 V range. The dc amplifier gain is set to X10. The measure customer (MC) input is connected to the internal TSENSE source which produces 0.6 volts. A 20 ms ADC measurement is performed and checked against a limit of $0.6\text{ V} \pm 0.3\text{ V}$.
- 611 DC gain x100 failed** This test configures for the 100 mV range. The dc amplifier gain is set to X100. The measure customer (MC) input is connected to the internal TSENSE source which produces 0.6 volts. A 20 ms ADC measurement is performed and checked for a + overload response.
- 612 Ohms 500 nA source failed** This test configures to the 10 V dc range with the internal 10 M 100:1 divider A4U102 connected across the input. the 500 nA Ohms current source is connected to produce a nominal 5 V signal. A 20 ms ADC measurement is performed and the result is checked against a limit of $5\text{ V} \pm 1\text{ V}$.
- 613 Ohms 5 μ A source failed** This test configures the 10 V range with the internal 10 M 100:1 divider A4U102 connected across the input. The 5 μ A current source is connected. The compliance limit of the current source is measured. A 20 ms ADC measurement is performed and the result is checked against a limit of $7.5\text{ V} \pm 3\text{ V}$.
- 614 DC 300V zero failed** This test configures the 300 V dc range with no input applied. A 20 ms ADC measurement is performed and the result is checked against a limit of $0\text{ V} \pm 5\text{ mV}$.

- 615 Ohms 10 μ A source failed** This test configures the 10 V range with the internal 10 M 100:1 divider A4U102 connected across the input. The 10 μ A current source is connected. A 20 ms ADC measurement is performed and the result is checked against a limit of $7.5\text{ V} \pm 3\text{ V}$.
- 616 DC current sense failed** This test configures the 1 A dc range and function. A 20 ms ADC measurement is performed and the result is checked against a limit of $0\text{ A} \pm 5\text{ A}$. This test confirms that the dc current sense path is functional.
- 617 Ohms 100 μ A source failed** This test configures the 10 V range with the internal 10 M 100:1 divider A4U102 connected across the input. The 100 μ A current source is connected. The compliance limit of the current source is measured. A 20 ms ADC measurement is performed and the result is checked against a limit of $5\text{ V} \pm 1\text{ V}$.
- 618 DC high voltage attenuator** This test configures to the 300 Vdc range. the 500 nA ohms current source is connected to produce a nominal 5 V signal. A 20 ms ADC measurement is performed and the result is checked against a limit of -10 mV to 70 mV at the output of the rms-to-dc converter.
- 619 Ohms 1 mA source failed** This test configures the 10 V range with the internal 10 M 100:1 divider A4U102 connected across the input. The 1 mA current source is connected. A 20 ms ADC measurement is performed and the result is checked against a limit of $7\text{ V} \pm 3.5\text{ V}$.
- 620 AC rms zero failed** This test configures to the 100 mV ac range with the ac input grounded through A4K103. The internal residual noise of the ac section is measured and checked against a limit of -10 mV to 70 mV at the output of the rms-to-dc converter.
- 621 AC rms full scale failed** This test configures for the 100 mV ac range. the 1 mA ohms current source is switched on the charge the ac input capacitor A4C301. This produces a pulse on the output of the rms-to-dc converter which is sampled 100 ms after the current is applied. A 20 ms A/D measurement is performed and checked against a limit of $10\text{ V} \pm 8.5\text{ V}$ into the ADC.

- 622 Frequency counter failed** This test configures for the 100 mV ac range. This test immediately follows test 621. With A4C301 holding charge from test 621 the ac input is now switched to ground through A4K103. This produces a positive pulse on the input to the frequency comparator A4U310. While C301 discharges, the ENAB FREQ bit is toggled four times to produce a frequency input to the counter logic in A1U205. A failure occurs if the counter can not measure the frequency input.
- 623 Cannot calibrate precharge** This test configures to the 100 V dc range with no input. The ADC is configured for 200 ms measurements. The A1U205 pulse width modulated (PWM) DAC output (C224) is set to about 4 volts. A reading is taken in with A4U101 in the MC state. A second reading is taken in the PRE state. The precharge amplifier voltage offset is calculated. The A1U205 DAC output is set to about 1.5 volts and the precharge offset is measured again. The gain of the offset adjustment is calculated. This test assures a precharge amplifier offset is achievable.
- 624 Unable to sense line frequency** This test checks that the LSENSE logic input to A1U205 is toggling. If no logic input is detected, the meter will assume a 50 Hz line operation for all future measurements.
- 625 I/O processor did not respond** This test checks that communications can be established between A1U205 and A1U305 through the optically isolated (A1U213 and A1U214) serial data link. Failure to establish communication in either direction will generate an error. If this condition is detected at power-on self-test, the instrument will beep and the error annunciator will be on.
- 626 I/O processor failed self-test** A failure occurred when the earth referenced processor, AU305, executed an internal RAM test.

Battery Check and Replacement


The internal battery, A1BT101, provides power to the internal real-time clock, stored states, and reading storage memory whenever ac line power is removed.

Note: *The internal battery state does not affect the calibration memory.*

The battery has an expected life of approximately 4 years. Battery life will be reduced if the instrument is stored for prolonged periods at temperatures above 40 °C with the ac power removed. The battery is not used whenever the ac line power is applied to the instrument.

The internal battery may be monitored to verify operation as described below. A low battery will typically give errors when ac line power is removed and then re-applied. Any of the following errors may indicate a low battery:


- 201, "Memory lost: stored state"
- 202, "Memory lost: power-on state"
- 203, "Memory lost: stored readings"
- 204, "Memory lost: time and date"

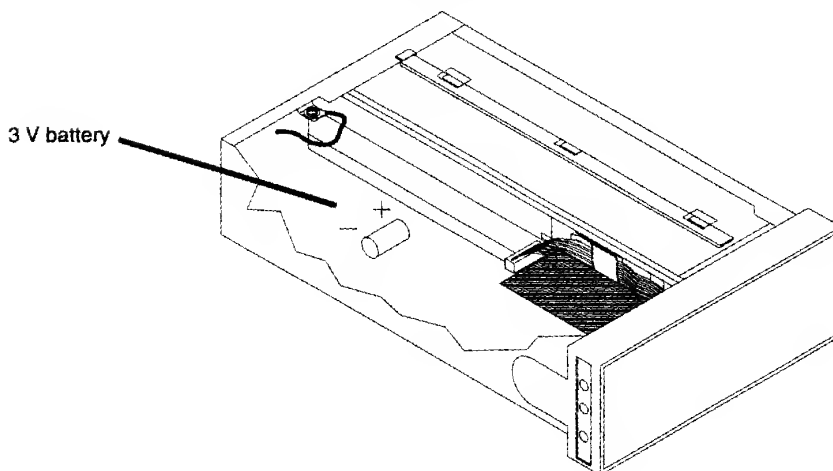

Properly dispose
of lithium battery.

To verify the battery:


- 1 Remove AC line power (this also provides a load on A1BT101).
- 2 Remove the cover (see page 156).
- 3 Measure the battery voltage as shown. Replace the battery if the voltage is below 2.7 V.

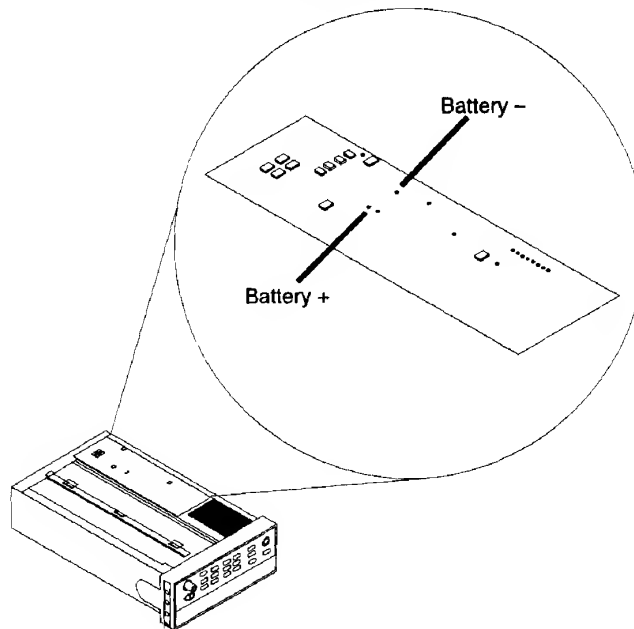



To replace the battery:

- 1 Remove AC line power.
- 2 Remove the cover (see page 156). If installed, remove the Internal DMM (A4) assembly (see page 158).
- 3 Turn the instrument over and unsolder the three battery terminals from the bottom of the circuit board. Use proper through-hole soldering techniques and equipment. Remove the battery, dispose of properly.
- 4 Install, solder and verify the new battery.


General Disassembly

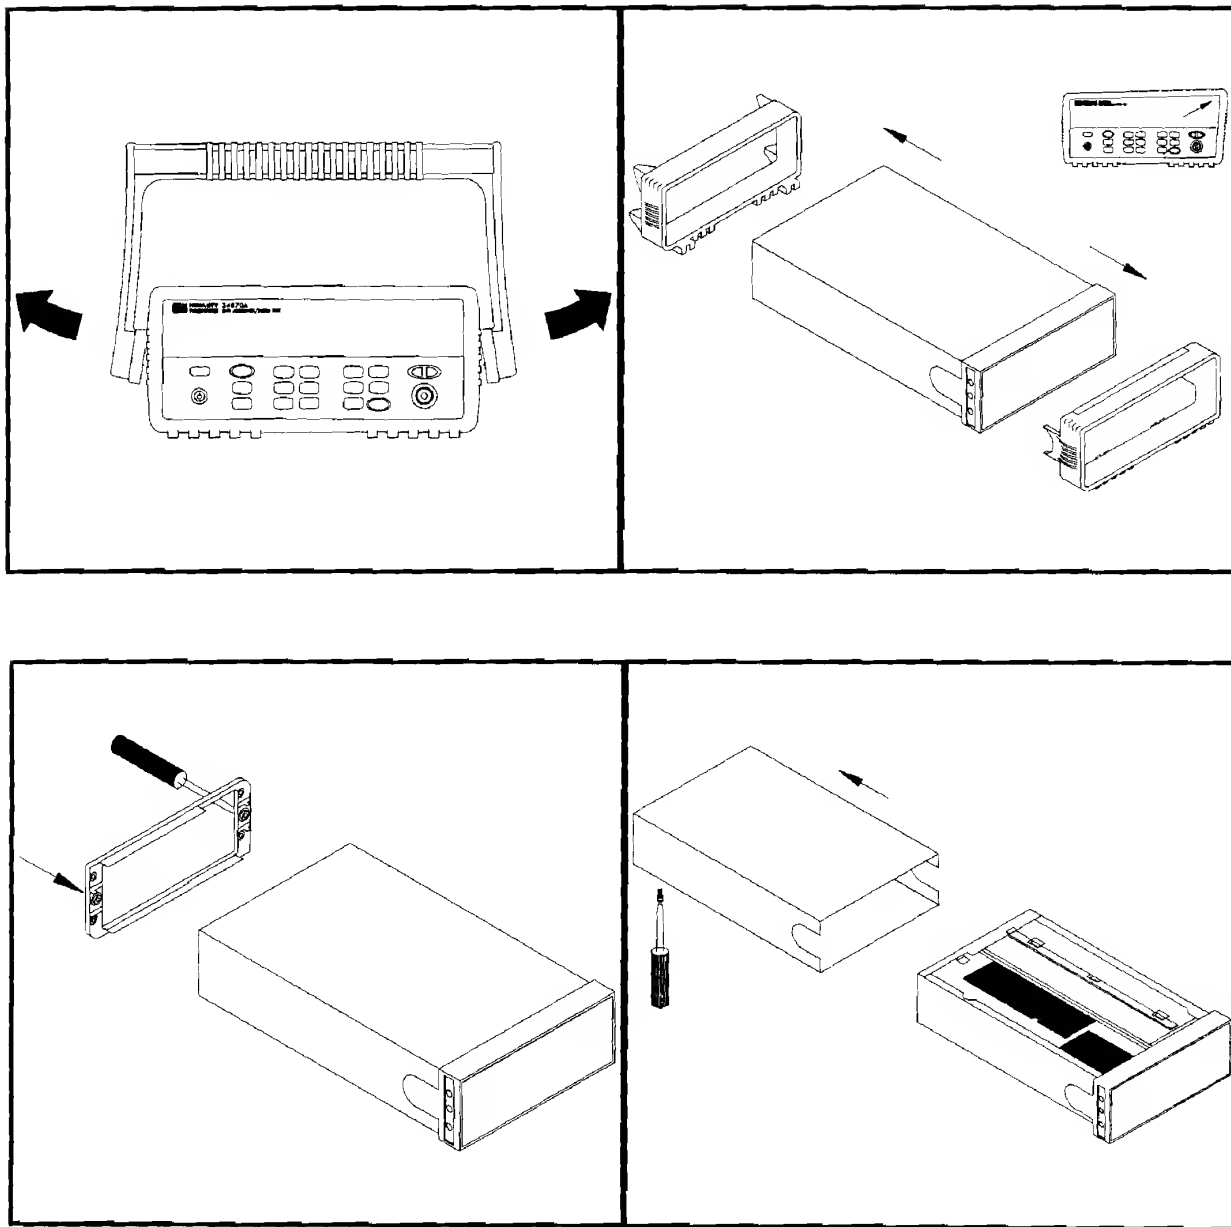


Internal DMM Disassembly

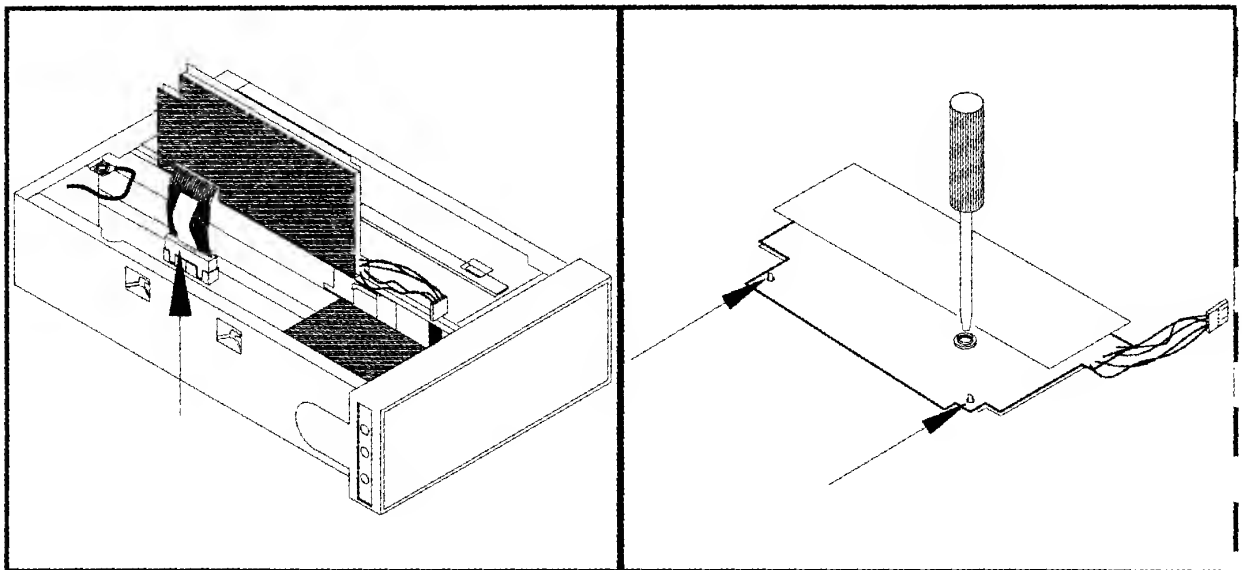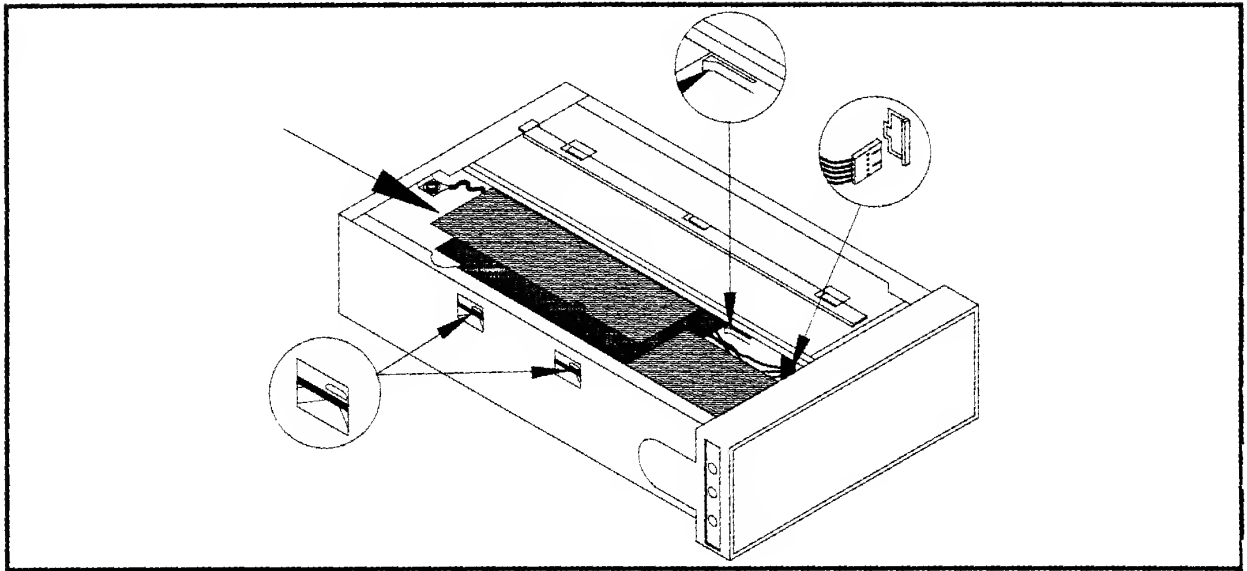



Front Panel Disassembly

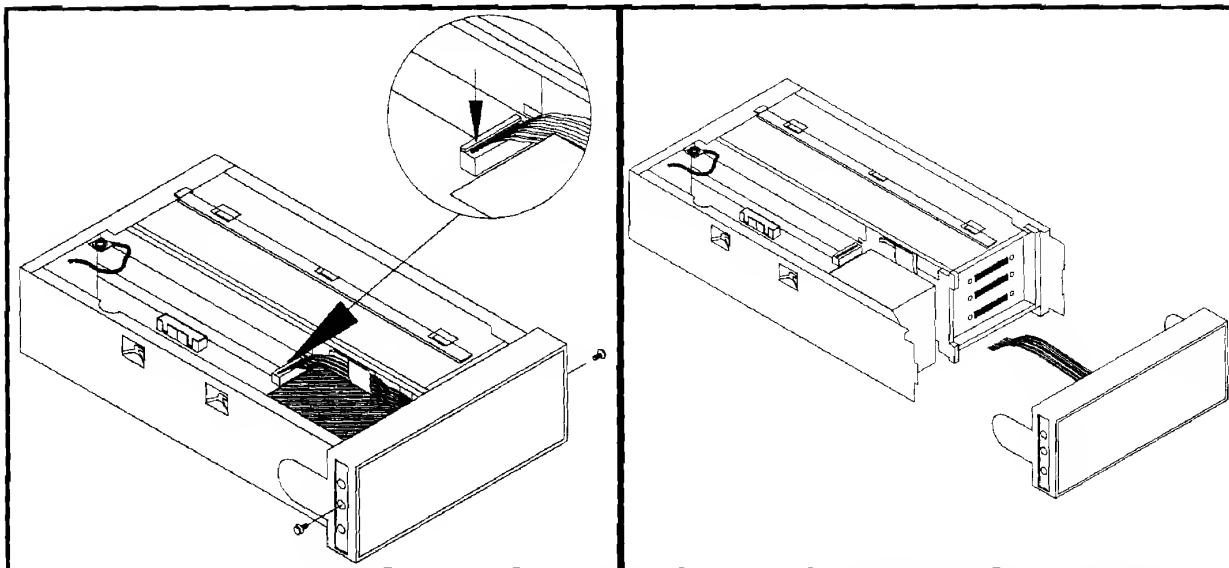


Note When reassembling, route the front panel cable as shown. Do not allow the front panel cable to touch the digital cable.

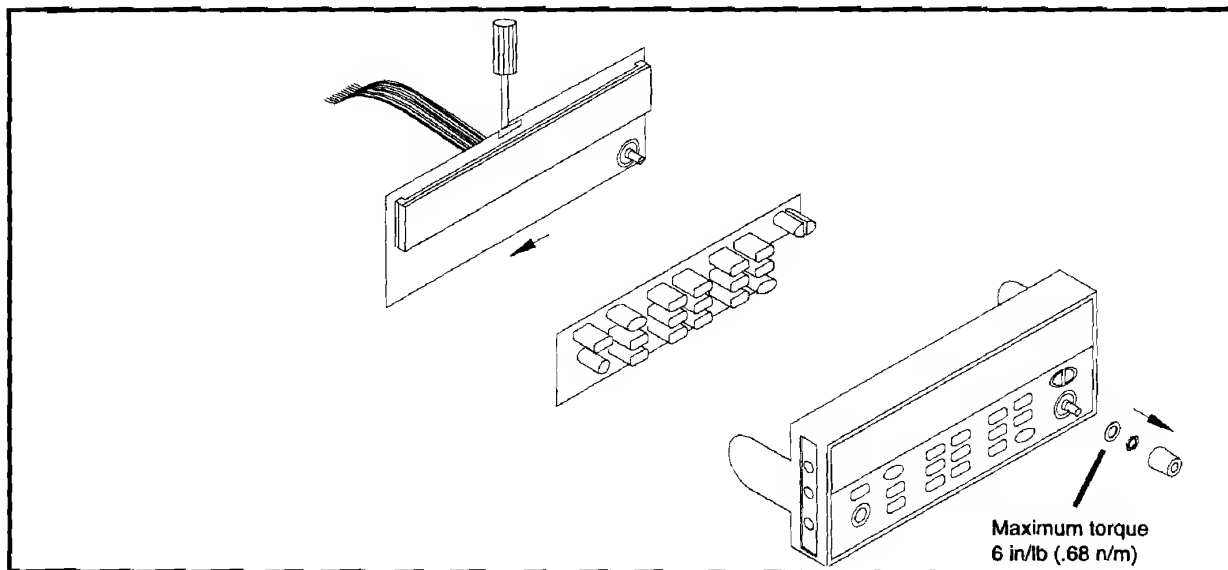

Additional Disassembly

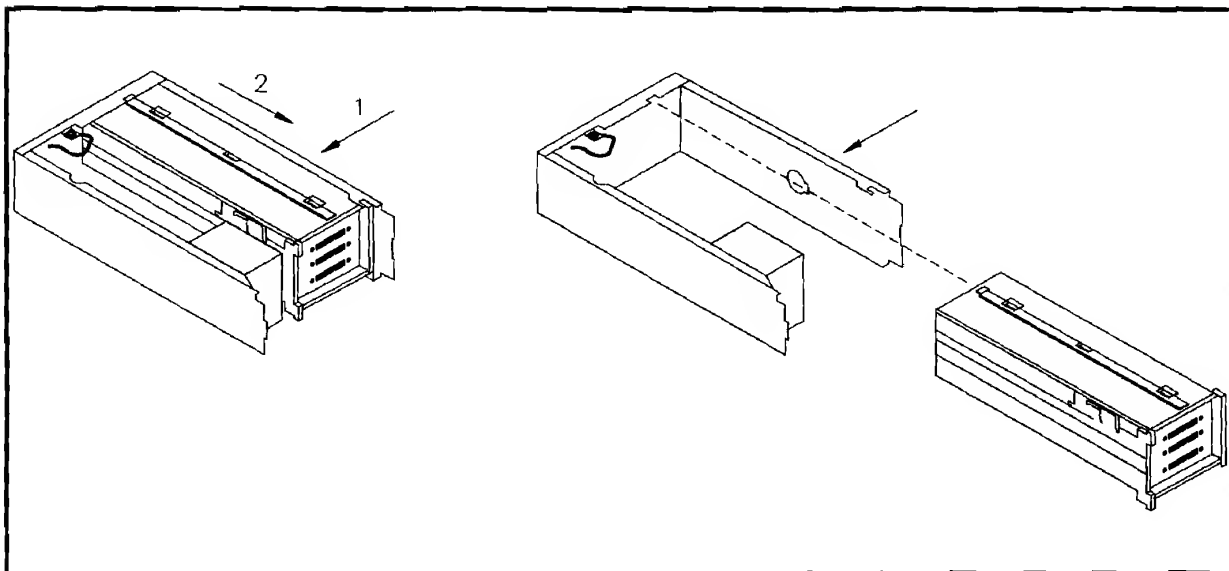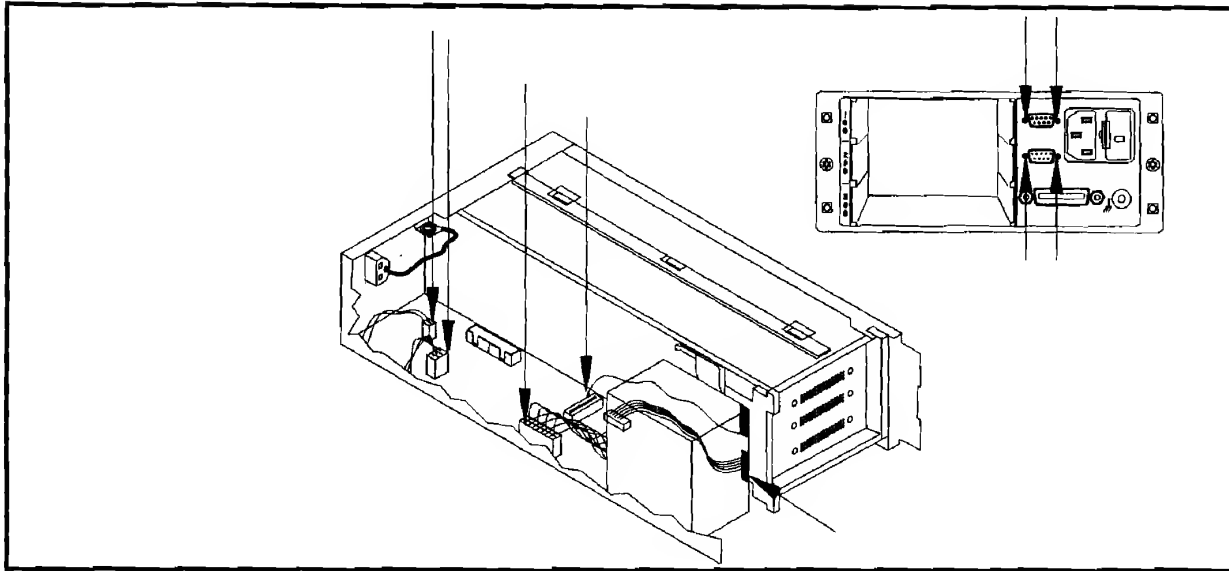

Plug-in Module Disassembly

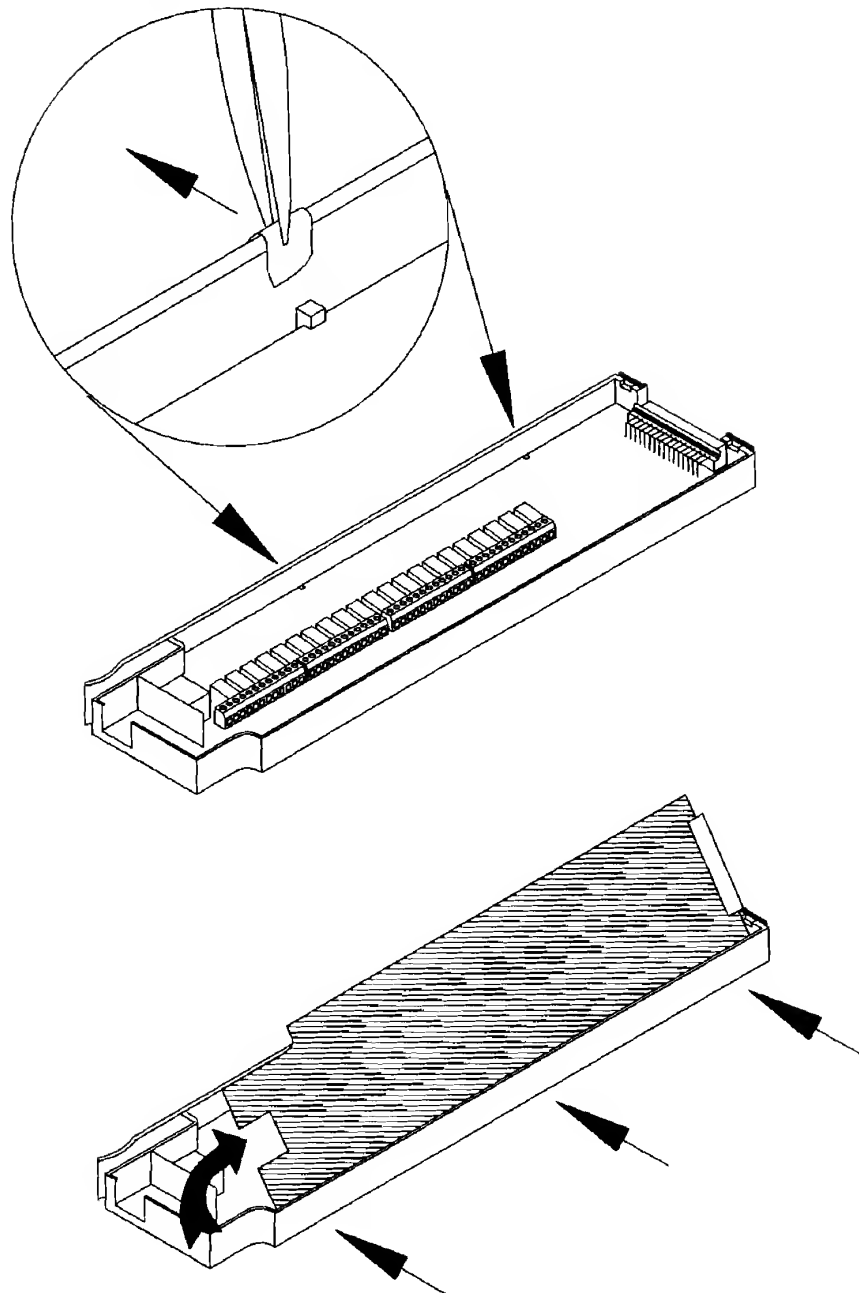

Replaceable Parts

Replaceable Parts

This chapter contains information ordering replacement parts for your instrument. The parts lists are divided into the following groups.

- HP 34970 Mainframe, *on page 165*
- 34970-66501 A1 PC Assembly, *on page 166*
- 34970-66502 A2 PC Assembly, *on page 171*
- 34970-66503 A3 PC Assembly, *on page 172*
- 34970-66504 A4 PC Assembly, *on page 173*
- HP 34901A 20-Channel Multiplexer, *on page 178*
- HP 34902A 16-Channel Multiplexer, *on page 181*
- HP 34903A 20-Channel Actuator Rev B, *on page 183*
- HP 34904A 4x8 Matrix, *on page 185*
- HP 34905A/34906A RF Multiplexer, *on page 188*
- HP 34907A Multifunction Module, *on page 190*
- HP 34908A 40-Channel Multiplexer, *on page 194*
- Manufacturer's List, *on page 197*

Parts are listed in alphanumeric order according to their schematic reference designators. The parts lists include a brief description of the part with applicable HP part numbers and manufacturer part number.

To Order Replace Parts

You can order replaceable parts from Hewlett-Packard using the HP part number or directly from the manufacturer using the manufacturer's part number. To order replaceable parts from HP, do the following:

- 1 Contact your nearest HP Sales Office or HP Service Center.
- 2 Identify the parts by the HP part number shown in the replaceable parts list. Note that not all parts are directly available from HP; you may have to order certain parts from the specified manufacturer.
- 3 Provide the instrument model number and serial number.

Backdating and Part Changes

Always refer to chapter 8, "Backdating" before attempting repair or before ordering replacement parts. Parts changes are documented in the backdating chapter.

Chapter 7 Replaceable Parts
HP 34970 Mainframe

HP 34970 Mainframe

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
A1	34970-66501	1	PCA-DIGITAL BD	02362	34970-66501
A2	34970-66502	1	PCA-DISPLAY BD	02362	34970-66502
A3	34970-66503	1	PCA-BACKPLANE BD	02362	34970-66503
A4	34970-66504	1	PCA-DMM BD	02362	34970-66504
CBL1	34970-61606	1	CABLE, K-TYPE TC, SCRWDRVR	02362	34970-61606
CBL2	5182-4794	1	CABLE, RS232, 9 PIN	02362	5182-4794
CBL3	8120-1378	1	CBL-U.S.	04940	07913-008GY
CVR1	34970-84101	1	COVER-SHEET METAL	02361	34970-84101
FRM1	34970-80101	1	CHASSIS	02361	34970-80101
HDW1	0535-0154	1	NUT HEX 11mm X2t	11239	37689
HDW2	3050-1941	1	WASHER-FL NM 7/16 IN .353-IN-ID	05227	.593+-005X.353+-005X.032+-003
MNL1	34970-90100	1	MANUAL SET	02362	34970-90100
MP1	34401-45011	1	HANDLE-FRONT	02362	34401-45011
MP2	34401-86010	1	KIT-BUMPERS/COVER	02362	34401-86010
MP3	34970-00101	1	CARD CAGE, LEFT	02362	34970-00101
MP4	34970-00102	1	CARD CAGE, RIGHT	02362	34970-00102
MP5	34970-40201	1	FRNT PANEL ASSY	02362	34970-40201
MP6	34970-44111	2	COVER PLATE, PLASTIC	02362	34970-44111
MP7	34970-49301	1	WINDOW/FRONT	02362	34970-49301
MP8	34970-68501	1	FAN	02362	34970-68501
MP9	34970-86201	1	PWR MOD W/FUSE	02362	34970-86201
MP10	34970-87401	1	KNOB	02362	34970-87401
MP11	34970-88001	1	KEYPAD	02362	34970-88001
MP12	34970-88301	1	BEZEL-REAR, MLD	02362	34970-88301
SCW1-SCW7	0515-0433	7	SCRPHM4.0X08TXSC	02361	0515-0433
SCW8-SCW9	0624-0751	2	SCR 6-19X1/2TORX	05610	225-23290-890-04
SHD1	34970-00601	1	SHIELD-XFMR	02361	34970-00601
SHD2	34970-00602	1	SHIELD-AC LINE	02361	34970-00602
SHD3	34970-00603	1	SHIELD-DMM	02362	34970-00603
T1	9100-5608	1	XFMR-PWR 100/120/220/240V	02859	14-7522

7

Chapter 7 Replaceable Parts
34970-66501 A1 PC Assembly

34970-66501 A1 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
BT101	5021-2000	1	BATTERY 3V .65A-HR LITHIUM POLYCARBON	08709	BR-1/2AE2SP
C101	0180-4435	3	CAP-FXD 2200uF +-20% 25 V AL-ELCTLT	06360	KME25VB222M16X25MCV
C102	0180-4558	1	CAP-FXD 33uF +-20% 20 V TA	12340	T491D336M020AS
C103	0160-7798	24	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C104	0180-4435		CAP-FXD 2200uF +-20% 25 V AL-ELCTLT	06360	KME25VB222M16X25MCV
C105-C106	0180-4116	3	CAP-FXD 22uF +-20% 20 V TA	00039	NRD226M20R12
C107	0180-4433	2	CAP-FXD 1000uF +-20% 50 V AL-ELCTLT	06360	KME50VB102M16X25MCV
C108	0180-3751	2	CAP-FXD 1uF +-20% 35 V TA	00039	NRS105M35R8
C109	0180-4433		CAP-FXD 1000uF +-20% 50 V AL-ELCTLT	06360	KME50VB102M16X25MCV
C110	0180-3751		CAP-FXD 1uF +-20% 35 V TA	00039	NRS105M35R8
C112-C116	0160-5945	9	CAP-FXD 0.01uF +-10% 50 V CER X7R	02010	08055C103KATA
C121	0180-4435		CAP-FXD 2200uF +-20% 25 V AL-ELCTLT	06360	KME25VB222M16X25MCV
C132	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C151	0180-4116		CAP-FXD 22uF +-20% 20 V TA	00039	NRD226M20R12
C160	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C180-C183	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C201	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C204-C205	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C209	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C212-C214	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C218	0160-5945		CAP-FXD 0.01uF +-10% 50 V CER X7R	02010	08055C103KATA
C219	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C220	0180-3744	1	CAP-FXD 4.7uF +-20% 10 V TA	00039	NRS475M10R8
C221	0160-5945		CAP-FXD 0.01uF +-10% 50 V CER X7R	02010	08055C103KATA
C222-C223	0160-5957	3	CAP-FXD 47pF +-5% 50 V CER C0G	03292	0160-5957
C224	0180-4228	1	CAP-FXD 47uF 10 V TA	05524	293D476X00101D2W
C270-C272	0160-5947	6	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C290-C292	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C301-C312	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C313	0160-5951	1	CAP-FXD 47pF 50 V	02010	08055A470JATA
C314	0160-5946	1	CAP-FXD 3300pF 50 V	02010	08051C332KATA
C315	0160-5961	1	FIXED CAPACITOR; 22PF 50 VOLTS	02010	08055A220JATA
C316	0160-5957		CAP-FXD 47pF +-5% 50 V CER C0G	03292	0160-5957
C317-C320	0180-4287	4	CAP-FXD 10uF +-20% 35 V TA	05524	293D106X0035D2W
C330-C331	0160-5947		CAP-FXD 1000pF 50 V	02010	08055C102KATA
C350-C351	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C370	0160-5947		CAP-FXD 1000pF 50 V	02010	08055C102KATA
C373	0160-5945		CAP-FXD 0.01uF +-10% 50 V CER X7R	02010	08055C103KATA

Chapter 7 Replaceable Parts
34970-66501 A1 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C401-C409	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C410	0160-5945		CAP-FXD 0.01uF +-10% 50 V CER X7R	02010	08055C103KATA
CR101-CR10	1901-1375	4	DIODE, 3A, 400V, 75NS, NON-PHOTOSENSITIVE	02037	MURS340
CR105	1906-0407	2	DIODE-FW BRDG 400V 1A	12810	DB104S
CR106-CR10	1902-1609	2	DIODE-ZNR 6.2V 5% PD=1.5W IR=5UA	02037	1SMB5920B
CR108	1902-1512	1	DIODE-ZNR 7.5V 5% TO-236 (SOT-23)	02910	BZX84C7V5
CR109	1906-0407		DIODE-FW BRDG 400V 1A	12810	DB104S
CR110	1906-0291	12	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR201-CR20	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR301-CR310	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
E102	9170-1584	15	CORE-SHLD BEAD	09808	25Z0805-0SR
E103	1205-0686	3	HEAT SINK SGL TO-220-CS	07179	576802B04000
E105-E106	1205-0686		HEAT SINK SGL TO-220-CS	07179	576802B04000
E120-E124	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
E201	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
E202-E203	9170-1506	2	CORE-MAGNETIC	06352	HF50ACB201209
E204	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
E206-E208	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
E301	9170-1663	1	CORE-SHIELDING BEAD	11702	FBM4532HM132
E315-E318	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
J201	1252-4484	1	CONN-POST TYPE 2.0-PIN-SPCG 12-CONT	03418	52007-1210
J202	1252-8542	1	CONN FRCC VERT MALE 26PIN	04726	2526-6302
J302	1252-2161	1	CONN-RECT MICRORBN 24-CKT 24-CONT	01380	554923-2
MAJ302	2190-0577	2	WASHER- NO. 10 .194-IN-ID .294-IN-OD	02361	2190-0577
MAU101	1205-1178	1	HEAT SINK	02361	1205-1178
MBJ302	2190-0577		WASHER- NO. 10 .194-IN-ID .294-IN-OD	02361	2190-0577
MCJ302	0380-0643	2	STANDOFF-HEX .255-IN-LG 6-32-THD	02361	0380-0643
MDJ302	0380-0643		STANDOFF-HEX .255-IN-LG 6-32-THD	02361	0380-0643
P101	1252-4487	1	CONN-POST TYPE .156-PIN-SPCG 3-CONT	03418	26-64-4030
P102	1252-4488	1	CONN-POST TYPE .156-PIN-SPCG 8-CONT	03418	26-64-4080
P110	1251-5066	1	CONN-POST TYPE 2.5-PIN-SPCG-MTG-END	03418	22-04-1021
P201	1251-0600	1	CONNECTOR-SGL CONT PIN 1.14-MM-BSC-SZ SQ	01136	928-196-004140
P302	34970-61601	1	CABLE, DGTL-BKPLN	03418	22-43-2060
P303	34970-61602	1	CABLE, RS232-DGTL	04726	87920-1000T
Q101	1855-1101	1	TRANSISTOR-MOSFET DUAL P-CHAN E-MODE SI	02037	MMDF2P02E
Q102	1854-1037	1	TRANSISTOR NPN SI TO-236AA PD=350MW	02237	MMBT3904
Q110	1855-0926	1	FET NMOS 2X S0BN 30V 1.5A R MMDF1N05	02037	MMDF1N05E

**Chapter 7 Replaceable Parts
34970-66501 A1 PC Assembly**

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q120	1853-0724	1	TRANSISTOR PNP SI TO-261AA (SOT-223)	06121	PZT2907A
R101	0699-2643	5	RESISTOR 0 +5% .1W TKF TC=0+-300	06337	9C08052A0R00JL
R102	0699-2990	2	RESISTOR 42.2K +-1% .1W TKF TC=0+-100	06337	9C08052A4222FKR
R103	0699-2643		RESISTOR 0 +5% .1W TKF TC=0+-300	06337	9C08052A0R00JL
R104	0699-2990		RESISTOR 42.2K +-1% .1W TKF TC=0+-100	06337	9C08052A4222FKR
R105-R106	0699-3051	9	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R107	0699-3060	2	RESISTOR 237 +-1% .1W TKF TC=0+-100	06337	9C08052A2370FKR
R108	0699-3740	1	RESISTOR 3.32K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-3321
R109	0699-2643		RESISTOR 0 +5% .1W TKF TC=0+-300	06337	9C08052A0R00JL
R110	0699-3060		RESISTOR 237 +-1% .1W TKF TC=0+-100	06337	9C08052A2370FKR
R111	0699-3040	1	RESISTOR 3.16K +-1% .1W TKF TC=0+-100	02995	9C08052A3161FKR
R112	0699-2643		RESISTOR 0 +5% .1W TKF TC=0+-300	06337	9C08052A0R00JL
R114-R115	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R118-R120	0699-3053	31	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R130-R131	0699-3034	17	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R132	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R201	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R202	0699-2965	13	RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R203	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R206	0699-3058	20	RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R208-R209	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R210	0699-3001	1	RESISTOR 215K +-1% .1W TKF TC=0+-100	06337	9C08052A2153FKR
R211	0699-3819	1	RESISTOR 10M +5% .1W TKF TC=0+-100	05524	CRCW08051005J
R212	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R213	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R214	0699-2983	1	RESISTOR 5.62K +-1% .1W TKF TC=0+-100	06337	9C08052A5621FKR
R215-R216	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R217	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R219-R220	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R221	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R222	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R251	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R252-R254	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R255	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R256	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R257-R259	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R260	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R261	0699-2965		RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R262	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R270	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR

Chapter 7 Replaceable Parts
34970-66501 A1 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R271-R273	0699-2977	6	RESISTOR 681 +-1% .1W TKF TC=0+-100	06337	9C08052A6810FKR
R280	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R301-R302	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R303	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R304	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R305-R309	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R310	0699-3034	1	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R311	0699-3050		RESISTOR 100K +-1% .1W TKF TC=0+-100	06337	9C08052A9091FKR
R312	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R313	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	06337	9C08052A1004FKR
R314	0699-3035	1	RESISTOR 1.47K +-1% .1W TKF TC=0+-100	06337	9C08052A1471FKR
R315	0699-3034	1	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R330-R331	0699-2977		RESISTOR 681 +-1% .1W TKF TC=0+-100	06337	9C08052A6810FKR
R340	0699-2965		RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R350	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R351-R354	0699-2965		RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R355-R358	0699-2965		RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R360-R362	0699-3058		RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R370	0699-2977		RESISTOR 681 +-1% .1W TKF TC=0+-100	06337	9C08052A6810FKR
R371-R372	0699-2965		RESISTOR 46.4K +-1% .1W TKF TC=0+-100	06337	9C08052A4642FKR
R373	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R375	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R380	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R401	0699-2643		RESISTOR 0 +5% .1W TKF TC=0+-300	06337	9C08052A0R00JL
R403-R423	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
U101	1826-2794	1	IC V RGLTR-FXD-POS 4.85/5.15V 3-TO-220	03406	LM2490CT-5.0-LB01
U102	1826-2264	1	IC PWR MGT-UND-V-SEN 8 PINS P-SOIC PKG	02037	MC34064D-5
U103	1826-1597	1	IC PWR MGT-V-REG-FXD-POS 4.85/5.15V	03406	LM2940CT-5.0
U104	1826-3044	1	IC PWR MGT-VS-SUPVR/CONT 16 PINS P-SOIC	03285	ADM691AR
U105	1826-0393	1	IC PWR MGT-V-REG-ADJ-POS 1.2/37V 3 PINS	01698	LM317KC
U106	1826-0527	1	IC PWR MGT-V-REG-ADJ-NEG 1.2/37V 3 PINS	03406	LM337T
U107	1826-1572	1	IC COMPARATOR PRCN DUAL 8 PIN PLSTC-SOIC	02910	LM393D
U150	1826-2817	1	IC PWR MGT-V-REF-FXD 4.975/5.025V 3 PINS	03406	LM4040CIM3-5.0
U201	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U204	1813-0827	1	CLK-OSC-XTAL STD 12.000-MHZ 0.01%	12768	SG-615P-12.000MC
U205	1821-1479	1	IC-80C196	03811	N80C196KB16
U209	1821-2271	1	ASIC 0.8U GATE ARRAY PERIPH/MEM CONTROL	03677	6559.024
U212	1820-5937	1	IC FF CMOS/AC D-TYPE POS-EDGE-TRIG	03406	74AC74SC
U213-U214	1990-1552	4	OPTO-ISOLATOR LED-IC GATE IF=10MA-MAX	01542	HCPL-2211-300
U215	9164-0173	1	ALARM-AUDIBLE PIEZO ALARM PIN TYPE; 25V	09939	PKM22EPP-4002S

Chapter 7 Replaceable Parts
34970-66501 A1 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
U220	1821-3433	1	7S14-SINGLE GATE, INVERTER, SCHMIT TRIGTNY	03406	NC7S14M5
U301	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07
U302	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U303	1990-1552		OPTO-ISOLATOR LED-IC GATE IF=10MA-MAX	01542	HCPL-2211-300
U304	1820-7312	3	IC SCHMITT-TRIG CMOS/ACT INV HEX	02037	MC74ACT14DR2
U305	34970-88803	1	PROG PART LOWER LEVEL 1821-1876		
U306	1820-7312		IC SCHMITT-TRIG CMOS/ACT INV HEX	02037	MC74ACT14DR2
U307	1820-6863	1	IC-UART WITH FIFO	03406	PC16550DV
U308	1820-6823	1	IC-INTERFACE DRVVR/RCVR CMOS TPL -888-BIT	02037	MC145407DW
U309	1821-1721	1	IC-HPIB CONTROLLER	01698	MP9914FNL
U310	1820-6175	1	IC-INTERFACE XCVR BIPOLAR BUS OCTL	01698	SN75ALS162DW
U311	1820-6176	1	IC-INTERFACE XCVR BIPOLAR BUS OCTL	01698	SN75ALS160DW
U312	1990-1552		OPTO-ISOLATOR LED-IC GATE IF=10MA-MAX	01542	HCPL-2211-300
U320	1820-7312		IC SCHMITT-TRIG CMOS/ACT INV HEX	02037	MC74ACT14DR2
U401	34970-88801	1	OTP - PROG 1820-8905		
U402-U405	1818-6000	4	IC 1M-BIT SRAM 70-NS CMOS	06916	CXK581000AM-70SL
U410	1818-5917	1	IC 256K-BIT SRAM 70-NS CMOS	06916	CXK58257AM-70LL (UNPRGMD)
Y201	0410-2153	1	CRYSTAL-QUARTZ 32.768 KHZ	10421	MC-405, 32.768K
Y301	0410-2622	1	CRYSTAL-QUARTZ 3.6864 MHZ	09235	FPX0368-20

34970-66502 A2 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C1	0180-3751	1	CAP-FXD 1uF +-20% 35 V TA	00039	NRS105M35R8
C2	0180-4287	1	CAP-FXD 10uF +-20% 35 V TA	05524	293D106X0035D2W
C3-C13	0160-7798	11	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
CR1	1902-1542	1	DIODE-ZNR 6.2V 5% TO-236 (SOT-23)	02037	BZX84C6V2
CR2	34970-89301	1	INDICATOR PANEL, VACUM FLOURESCENT DSPLY	11908	34970-89301
E1	34970-00604	1	SHIELD, ESD TEMP PART FOR ASSY34970-66502	02361	34970-00604
E2	9170-1506	1	CORE-MAGNETIC	06352	HF50ACB201209
J1	34970-61612	1	CABLE, DISPLAY	02632	34970-61612
R1	0699-3070	1	RESISTOR 26.1K +-1% .1W TKF TC=0+-100	06337	9C08052A2612FKR
R2	0699-3039	1	RESISTOR 2.61K +-1% .1W TKF TC=0+-100	06337	9C08052A2611FKR
R3-R4	0699-3053	2	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R5-R7	0699-3051	4	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R8-R10	0699-3058	3	RESISTOR 100 +-1% .1W TKF TC=0+-100	06337	9C08052A1000FKR
R11	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U1	34970-88811	1	PGM'D 1820-8905 8 BIT MCU W/4K EPROM	02632	34970-88811
U2	1826-1734	1	IC PWR MGT-V-REG-FXD-POS 4.8/5.2V 3 PINS	02037	MC78M05CDT
U3	0410-4009	1	CERO-RES 12MHZ +-1-0.8%	00830	PBRC-12.0BRN07
U4-U5	1820-5330	2	IC-INTERFACE DRVR BIPOLAR DISPLAY	01698	SN75518FN
U6	1826-1528	1	IC COMPARATOR LP QUAD 14 PIN PLSTC-SOIC	02037	LM339D
U7	1826-2264	1	IC 34064	02037	MC34064D-5
U8	0960-0961	1	ROTARY ENCODER 24POS TH-VERT	03744	ECLOJ-C24-SE002

Chapter 7 Replaceable Parts
34970-66503 A3 PC Assembly

34970-66503 A3 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C109	0160-7438	1	CAP-FXD 0.01uF +-10% 500 V CER X7R	02010	12107C103KATA
E101-E102	1970-0100	2	TUBE-ELECTRON SURGE V PTCTR	11484	1970-0100
J1	1400-0977	1	CLIP BAT	05535	209
L101-L102	9140-1194	2	INDUCTOR 10NH +-10% 2.8W-MMX3.4LG-MM	02366	KL32TE010K
P101-P103	1252-8025	3	CONN DIN VERT MALE 48PIN	02010	16-8477-048-001-025
P104	1252-3442	1	CONN-POST TYPE .100-PIN-SPCG 6-CONT	03418	705-55-0075
P105	1252-3441	1	CONN DIS RA M SPIN SMC	03418	705-55-0074
P106	34970-61611	1	BACKPLANE CABLE	00003	34970-61611
R101	0699-1327	1	RESISTOR 1M +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R160	0699-4820	1	RESISTOR 220 5% AXIA1 .5W TC=0+200PPM	05524	RNX-3/8N220RJM
RV101-RV102	0837-0509	2	DIO, MOV, OPERV=230VRMS, 17J, CU4032K230GK1	06121	SIOV-CU4032K230GK1

Chapter 7 Replaceable Parts
34970-66504 A4 PC Assembly

34970-66504 A4 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C100	0160-6839	1	CAP-FXD 470pF 630 V POLYP-FL	02995	703E1AD471PG631TX
C101-C103	0160-6842	3	CAP-FXD 220pF 630 V POLYP-FL	02995	703E1AD221PG631TX
C104	0160-6497	18	CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C105	0160-6731	4	CAP-FXD 1000pF 50 V	02010	12065C102KATA
C106-C107	0160-5967	4	CAP-FXD 100pF +-5% 50 V CER COG	03292	0160-5967
C108	0160-6736	7	CAP-FXD 0.01uF 50 V	02010	12065C103KATA
C110	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C111	0160-5967		CAP-FXD 100pF +-5% 50 V CER COG	03292	0160-5967
C113	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C120	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C150	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C151	0160-6736		CAP-FXD 0.01uF 50 V	02010	12065C103KATA
C152	0160-6731		CAP-FXD 1000pF 50 V	02010	12065C102KATA
C160	0160-6736		CAP-FXD 0.01uF 50 V	02010	12065C103KATA
C210	0160-5954	4	CAP 220PF 5% 50V	02010	08055A221JATA
C212	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C301	0160-6778	1	CAP 0.22uF 400 V	05176	HEW-671-220NF+/-10%400V
C302	0160-7605	1	CAP-FXD 1.8pF +-13.89% 1.5 kV CER COG	02010	MA30SA1R8CAA
C303	0160-6098	1	CAP-FXD 680pF +-5% 50 V CER COG	02010	12065A681JATA
C304	0160-5973	1	CAP-FXD 6.8pF 50 V	02010	08055A6R8DATA
C305	0160-6096	1	CAP-FXD 470pF +-5% 50 V CER COG	02010	12065A471JATA
C306	0160-5972	1	CAP-FXD 5.6pF +-8.93% 50 V CER COG	02010	08051A5R6DATA
C307	0160-5967		CAP-FXD 100pF +-5% 50 V CER COG	03292	0160-5967
C308-C310	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C313	0160-5955	1	CAP-FXD 68pF +-5% 50 V CER COG	12473	0160-5955
C314-C315	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C316	0160-5892	2	CAPACITOR-FXD .22UF +-10% 63VDC	05524	MKT1817422065
C317	0160-6729	1	CAP. FIXED. CER./CHIP	02010	12065C332KATA
C318	0160-5892		CAPACITOR-FXD .22UF +-10% 63VDC	05524	MKT1817422065
C319-C320	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C321	0160-5469	1	CAPACITOR-FXD 1UF +-10% 50VDC	10881	BF064D0105KDB
C322-C323	0180-4733	2	CAP-FXD 22uF +-20% 25 V TA	12340	T495X226M025AS
C324	0160-5959	2	CAP-FXD 33pF +-5% 50 V CER COG	02010	08055A330JATA
C326	0160-6731		CAP-FXD 1000pF 50 V	02010	12065C102KATA
C327	0160-5959		CAP-FXD 33pF +-5% 50 V CER COG	02010	08055A330JATA
C330	0180-4559	1	CAP-FXD 68uF +-20% 10 V TA	12340	T491D686M010AS
C350-C351	0160-6736		CAP-FXD 0.01uF 50 V	02010	12065C103KATA
C400-C402	0160-5954		CAP 220PF 5% 50V	02010	08055A221JATA
C403-C404	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA

Chapter 7 Replaceable Parts
34970-66504 A4 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C407-C408	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C410	0160-6497		CAP-FXD 0.1uF 25 V	02010	12065C104KATA
C441-C442	0160-6736		CAP-FXD 0.01uF 50 V	02010	12065C103KATA
C460	0160-6731		CAP-FXD 1000pF 50 V	02010	12065C102KATA
CR103	1902-1565	1	DIODE-ZNR 4.7V 5% TO-236 (SOT-23)	02910	BZX84-C4V7
CR110-CR113	1901-1607	4	DIODE-PWR RECT 400V DO-214AB	04733	S3G
CR201	1902-1565	1	DIODE-ZNR 4.7V 5% TO-236 (SOT-23)	02910	BZX84-C4V7
CR202	1901-1378	1	DIODE; HV RECTIFIER 1.6KV	04504	GP10Y
CR203	1902-1592	1	DIODE-ZNR 5.1V 5% TO-236 (SOT-23)	02037	BZX84C5V1
CR302-CR303	1906-0291	4	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR304-CR307	1902-1541	6	DIODE-ZNR 3.3V 5% TO-236 (SOT-23)	02037	BZX84C3V3
CR401-CR402	1902-1541		DIODE-ZNR 3.3V 5% TO-236 (SOT-23)	02037	BZX84C3V3
CR403-CR404	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
K102-K104	0490-1896	3	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L101	9140-1244	2	INDUCTOR 1MH +-5% 3.4W-MMX4.8LG-MM Q=30	05524	IMC-18121000.0UH+-5%
L102	9140-1238	3	INDUCTOR 10UH +-5% 2.8W-MMX3.4LG-MM Q=30	02366	KL32TE100J
L106	9140-1244		INDUCTOR 1MH +-5% 3.4W-MMX4.8LG-MM Q=30	05524	IMC-18121000.0UH+-5%
L110-L111	9140-1238		INDUCTOR 10UH +-5% 2.8W-MMX3.4LG-MM Q=30	02366	KL32TE100J
L401-L402	9170-1431	2	CORE-SHLD BEAD	06352	HF50ACB-453215
L404	9170-1506	1	CORE-MAGNETIC	06352	HF50ACB201209
L405-L407	9170-1584	3	CORE-SHLD BEAD	09808	25Z0805-0SR
P100	34970-61604	1	CABLE, DMM-DGTL	04726	87926-1000T
P101	34970-61603	1	CABLE, DMM-BKPLN	02362	34970-61603
Q104	1855-0752	2	TRANSISTOR J-FET N-CHAN D-MODE TO-236AA	03406	MMBF4392
Q150-Q153	1854-1014	4	TRANSISTOR NPN SI TO-236AA PD=350MW	04200	TMPT6429
Q201	1855-0752		TRANSISTOR J-FET N-CHAN D-MODE TO-236AA	03406	MMBF4392
Q202	1855-0863	1	TRANSISTOR J-FET P-CHAN D-MODE TO-236AA	02237	MMBF5461SEL
Q203-Q208	1853-0727	6	TRANSISTOR PNP SI SOT-23 (TO-236AB)	02037	MMBT6520L
Q211	1855-0865	1	TRANSISTOR J-FET N-CHAN D-MODE TO-236AA	03406	MMBF4117A
Q301	1855-0800	1	TRANSISTOR MOSFET N-CHAN E-MODE TO-252AA	02037	MTD3055EL
R103	0699-1380	4	RESISTOR 3.16K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R104	0699-4821	3	RESISTOR 75K 5% 2512 200V 1W TC=200	05524	CRCW2512753J
R105	0699-3406	3	RESISTOR 24K +-5% 1W TKF TC=0+-200	05524	CRCW2512243J

**Chapter 7 Replaceable Parts
34970-66504 A4 PC Assembly**

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R112-R113	0699-3053	2	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R114-R117	0699-2973	12	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R118	0699-1380		RESISTOR 3.16K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R119	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R121	0699-3413	1	RESISTOR 5 +-0.1% .125W TF TC=0+-10	02499	RC659R00
R122	0699-1329	2	RESISTOR 6.19K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R123	0699-4845	1	RESISTOR .10 1% RES3F 2W TC=25PPM/DEGC	05524	WSR-2 .1 +/-1%
R124	0699-3046	1	RESISTOR 6.19K +-1% .1W TKF TC=0+-100	06337	9C08052A6191FKR
R126-R127	0699-2986	3	RESISTOR 21.5K +-1% .1W TKF TC=0+-100	06337	9C08052A2152FKR
R130	0699-3067	1	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R131	0699-2986		RESISTOR 21.5K +-1% .1W TKF TC=0+-100	06337	9C08052A2152FKR
R150	0699-3051	2	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R151	0699-3029	1	RESISTOR 316 +-1% .1W TKF TC=0+-100	06337	9C08052A3160FKR
R170	0699-4821		RESISTOR 75K 5% 2512 200V 1W TC=200	05524	CRCW2512753J
R173	0699-3406		RESISTOR 24K +-5% 1W TKF TC=0+-200	05524	CRCW2512243J
R183	0699-3406		RESISTOR 24K +-5% 1W TKF TC=0+-200	05524	CRCW2512243J
R184	0699-4821		RESISTOR 75K 5% 2512 200V 1W TC=200	05524	CRCW2512753J
R196	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R197	0699-3049	1	RESISTOR 8.25K +-1% .1W TKF TC=0+-100	06337	9C08052A8251FKR
R198	0699-3034	1	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R201	0699-3404	1	RESISTOR 400K +-1% .125W TF TC=0+-2	06337	5023ZT400K0F
R202	0699-4416	1	RESISTOR 40K +-1% .5W MF TC=0+- .0031	05524	S102C40K000 1%
R203-R205	0699-1332	3	RESISTOR 196K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R207	0699-3038	1	RESISTOR 2.37K +-1% .1W TKF TC=0+-100	06337	9C08052A2371FKR
R290	0699-1374	3	RESISTOR 1.78K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R301-R302	0699-2469	2	RESISTOR 500K +-0.25% .25W TF TC=0+-5	09454	PR1/4TC5500K.25%
R303	0699-1307	1	RESISTOR 1.96K +-0.1% .1W TF TC=0+-5	02995	5023Z
R304	0699-0481	1	RESISTOR 200K +-1% .1W TF TC=0+-10	02995	5023Z
R305	0699-1374		RESISTOR 1.78K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R306	0699-1423	3	RESISTOR 215 +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R307	0699-1374		RESISTOR 1.78K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R308	0699-1423		RESISTOR 215 +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R309	0699-1329		RESISTOR 6.19K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R310	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R311-R312	0699-1412	3	RESISTOR 75K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R313	0699-1380		RESISTOR 3.16K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R314	0699-1398	5	RESISTOR 21.5K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R315	0699-1327	1	RESISTOR 1M +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R316	0699-1423		RESISTOR 215 +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R317	0699-1406	2	RESISTOR 42.2K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR

Chapter 7 Replaceable Parts
34970-66504 A4 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R318	0699-1318	4	RESISTOR 1K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R319	0699-1398		RESISTOR 21.5K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R320	0699-1427	1	RESISTOR 316 +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R321	0699-1382	1	RESISTOR 3.83K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R322	0699-1412		RESISTOR 75K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R323-R324	0699-1398		RESISTOR 21.5K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R325-R326	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R327	0699-1398		RESISTOR 21.5K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R398-R399	0699-1391	3	RESISTOR 10K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R403	0699-1391		RESISTOR 10K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R405	0699-1380		RESISTOR 3.16K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R406	0699-1330	1	RESISTOR 100K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R407-R408	0699-1318		RESISTOR 1K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R409	0699-1372	1	RESISTOR 1.47K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R420	0699-1389	1	RESISTOR 8.25K +-1% .125W TKF TC=0+-100	06337	9C12063A8251FKR
R421	0699-1318		RESISTOR 1K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R422	0699-1360	1	RESISTOR 46.4 +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R430	0699-1503	1	RESISTOR .05 +-100% TKF	02995	9C12063A00R0JLR
R440	0699-1406		RESISTOR 42.2K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R441	0699-1394	1	RESISTOR 14.7K +-1% .125W TKF TC=0+-100	04935	9C12063AFKR
R442	0699-2127	1	RESISTOR 36.5K +-1% .125W TKF TC=0+-100	05524	CRCW12063652F
R450-R451	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R460-R461	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
RV102	0837-0320	1	VOLTAGE SUPPRESSOR VMAC=230V, VMDC=300V	06121	S07K230
SCR101	0515-0433	1	SCREW- X 8MM-LG -HD	02361	0515-0433
SHD101	34970-00603	1	SHIELD-DMM	02361	34970-00603
U101	1SK6-0001	1	INTEGRATED CIRCUIT; ASCI	02632	1SK6-0001
U102	1NB4-5035	1	CUST R NET PKG, REPLACES 34401-67901	02632	1NB4-5035
U103	1826-2420	5	IC OP AMP LP DUAL 8 PIN PLSTC-SOIC	03285	AD706JR
U104	1855-0864	1	TRANSISTOR, JFET DUAL	03406	NPDSU406
U105	1826-2558	3	IC OP AMP WB SINGLE 8 PIN PLSTC-SOIC	02037	MC34081BD
U106	1826-1925	2	IC OP AMP LOW-NOISE SINGLE 8 PIN	03285	OP-27GS
U110	1826-2558		IC OP AMP WB SINGLE 8 PIN PLSTC-SOIC	02037	MC34081BD
U150	1820-8937	1	IC Gate-ARY CMOS	03406	SCX6B04AKP
U153	1826-2420		IC OP AMP LP DUAL 8 PIN PLSTC-SOIC	03285	AD706JR
U201	1826-2420		IC OP AMP LP DUAL 8 PIN PLSTC-SOIC	03285	AD706JR
U301	1826-2436	1	IC OP AMP WB 8 PIN PLSTC-SOIC	03406	LF356M
U302	1826-2339	1	IC: 8-BIT 16-P-SOIC CMOS	03285	AD7524JR

Chapter 7 Replaceable Parts
34970-66504 A4 PC Assembly

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
U303	1826-2437	3	IC OP AMP WB 8 PIN PLSTC-SOIC	03406	LF357M
U304	1826-1985	1	ANALOG SWITCH 4 SPST 16 -P-SOIC	02883	DG411DY
U305	1826-2437		IC OP AMP WB 8 PIN PLSTC-SOIC	03406	LF357M
U306	1826-1609	1	ANALOG SWITCH 4 SPST 16 -P-SOIC	03285	ADG211AKR
U307	1826-2558		IC OP AMP WB SINGLE 8 PIN PLSTC-SOIC	02037	MC34081BD
U308	1826-2445	1	RMS/DC 16-P-SOIC MISC	03285	AD637JR
U309	1820-5790	2	IC SHF-RGTR CMOS/HC SYNCHRO SERIAL-IN	02910	74HC4094D
U310	1826-1572	1	IC COMPARATOR PRCN DUAL 8 PIN PLSTC-SOIC	02910	LM393D
U311	1820-5790		IC SHF-RGTR CMOS/HC SYNCHRO SERIAL-IN	02910	74HC4094D
U312	1826-2437		IC OP AMP WB 8 PIN PLSTC-SOIC	03406	LF357M
U400-U401	1826-2420		IC OP AMP LP DUAL 8 PIN PLSTC-SOIC	03285	AD706JR
U402	1826-1991	1	IC OP AMP HS SINGLE 8 PIN PLSTC-SOIC	03285	AD711JR
U403	1826-1249	1	IC, V RGLTR-V-REF-FXD	10858	LM399AH(SEL)
U411	1821-3334	1	IC-AN-MUX 74HC4053D 3X2:1 SOURCE-RESTRIC	02910	74HC4053D
U420	1826-1925		IC OP AMP LOW-NOISE SINGLE 8 PIN	03285	OP-27GS
U450	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S

Chapter 7 Replaceable Parts
HP 34901A 20-Channel Multiplexer

HP 34901A 20-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C106	0160-7798	8	CAP 0.1 uF 50V 10% X7R 0805	02010	08055C104KAT_A
C107	0160-7708	1	CAP-FXD 1000pF +5% 50 V CER COG	12340	C0805C102J5GAC
C109	0160-7798		CAP 0.1 uF 50V 10% X7R 0805	02010	08055C104KAT_A
C110	0160-7828	1	CAP .1 uF 16V 10% X7R	02010	0603C104KAT
C119-C124	0160-5947	6	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C125-C128	0160-7845	5	CAP-FXD 180PF +5% 50 V CER COG	12340	C0603C181J5GAC
C130-C135	0160-7751	6	CAP-FXD 0.01 uF +10% 50 V CER X7R	12340	C0603C103K5RAC
C140-C141	0160-5945	11	CAP-FXD 0.01 uF 50 V	02010	08055C103KATA
C145	0160-7798		CAP 0.1 uF 50V 10% X7R 0805	02010	08055C104KAT_A
C150	0180-4545		CAP-FXD 4.7 uF +20% 20 V TA	12340	T491B475M020AS
C151-C152	0160-5945		CAP-FXD 0.01 uF 50 V	02010	08055C103KATA
C201-C207	0160-5945		CAP-FXD 0.01 uF 50 V	02010	08055C103KATA
CR102	1906-0395	5	DIODE-DUAL 75V TO-253	02910	BAS28
CR103-CR106	1902-1574	4	DIODE-ZNR 6.8V 6% TO-236 (SOT-23)	02910	BZX84C6V8
CR107	1906-0291	24	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR201-CR220	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR221-CR222	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
CR320-CR322	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR323-CR324	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
F501-F502	2110-0043	2	FUSE (INCH) 1.5A 250V NTD FE UL-LST	04703	312 01.5
HAF502	2110-0726	4	FUSEHOLDER-CLP-TYP	02603	1115-0597T
HB502	2110-0726		FUSEHOLDER-CLP-TYP	02603	1115-0597T
HCF501	2110-0726		FUSEHOLDER-CLP-TYP	02603	1115-0597T
HDF501	2110-0726		FUSEHOLDER-CLP-TYP	02603	1115-0597T
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J102-J104	0360-2624	4	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
J105	0360-2623	1	CONN TERMINAL BK RA FEM 4 PIN	13389	M1.040.0001.8
J106	0360-2624		CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
K401-K420	0490-1896	24	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K421	0490-1895	3	RLY-2C 2A 220V 60WATT 4.5V COIL	12921	G6S-2-DC4.5
K422	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K423	0490-1895		RLY-2C 2A 220V 60WATT 4.5V COIL	12921	G6S-2-DC4.5
K521	0490-1895		RLY-2C 2A 220V 60WATT 4.5V COIL	12921	G6S-2-DC4.5
K522-K524	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L101-L103	9170-1663	3	CORE-SHIELDING BEAD	11702	FBM4532HM132

Chapter 7 Replaceable Parts
HP 34901A 20-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
L105	9170-1584	12	CORE-SHLD BEAD	09808	25Z0805-0SR
L109-L115	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L150-L153	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L401-L402	9140-1638	2	INDUCTOR 10UH +10% -10% 2.7W-MMX3.4LG-MM	06352	NLC322522T-100K
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
Q101	1855-1101	1	TRANSISTOR	02037	MMDF2P02E
Q201	1854-1053	25	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q202-Q203	1853-0525	22	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q204	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q205	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q206-Q207	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q208-Q209	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q210	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q211	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q212-Q213	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q214	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q215	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q216-Q217	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q218	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q219	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q220-Q221	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q222-Q223	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q224	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q225	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q226-Q227	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q228	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q301-Q303	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q304	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q305	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q306	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q307	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q308	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q309	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q310	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q311	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q312	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q313	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q314	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q315	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A

Chapter 7 Replaceable Parts
HP 34901A 20-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q316	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q317	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q318	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q319	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
R102-R103	0699-3034	11	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R104	0699-3947	6	RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R105	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R106-R109	0699-3970	5	RESISTOR 10K +-1% .063W TKF TC=0+-200	06337	232270461003
R110-R112	0699-3974	3	Resistor 14.7K 1% 0603 50V .063W TC=200	06337	9C0603A1472FL
R113	0699-3970		RES 10K 1% .063W	06337	232270461003
R114-R115	0699-3067	2	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R117-R121	0699-2973	5	RES 215, FIXED THIN FILM	06337	9C08052A2150FKR
R147	0699-3051	49	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	06337	9C08052A1004FKR
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R150-R154	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R155-R158	0699-3947		RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R170-R180	0699-3963	11	RESISTOR 4.64K 1% 0603 50V .063W TC=200	06337	9C0603A4641FL
R181	0699-3947		RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R182-R183	0699-3932	4	RESISTOR 215 +-1% .063W TKF TC=0+-200	06337	9C0603A2150FL
R185-R186	0699-3932		RESISTOR 215 +-1% .063W TKF TC=0+-200	06337	9C0603A2150FL
R201-R228	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R301-R319	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U101	34901-88811	1	PRGM'D 1821-1876	01542	34901-88811
U102-U106	1820-5752	5	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U109	1820-5941	1	IC DCDR-DEMUXR CMOS/ACT BIN 8-TO-1-LINE	03406	74ACT138SC
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U150	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U151-U152	1821-2382	2	IC-DS1620S	12186	DS1620S
XU101	1200-1592		SOCKET-IC-PLCC 44-CONT SQUARE J-LEAD	01380	3-822275-1
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
HP 34902A 16-Channel Multiplexer

HP 34902A 16-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C104	0160-7798	4	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C105-C112	0160-5967	8	CAP-FXD 100PF 5% 0805	03292	0160-5967
C113	0160-7828	1	CAP .1UF 16V 10% X7R	02010	0603C104KAT
C120	0160-5947	1	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C125-C128	0160-7845	4	CAP FXD 180PF +-5% 50 V CER COG	12340	C0603C181J5GAC
C130-C135	0160-7751	6	CAP-FXD 0.01uF +-10% 50 V CER X7R	12340	C0603C103K5RAC
C140-C141	0160-5945	7	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C150	0180-4545	1	CAP-FXD 4.7uF +-20% 20 V TA	12340	T491B475M020AS
C151-C152	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C160-C162	0160-7708	3	CAP-FXD 1000pF +-5% 50 V CER COG	12340	C0805C102J5GAC
C212-C214	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
CR102	1906-0395	11	DIODE-DUAL 75V TO-253	02910	BAS28
CR103-CR106	1902-1574	4	DIODE-ZNR 6.8V 6% TO-236 (SOT-23)	02910	BZX84C6V8
CR107	1906-0291	1	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR201-CR210	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
CR211	1902-1572	1	DIODE-ZNR 15V 5% TO-236 (SOT-23) PD=.35W	02910	BZX84-C15
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J401-J403	0360-2624	3	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
K301-K316	0490-1897	19	RELAY-REED 2A 1A 300VDC 5VDC-COIL	04501	3500-0113
K326-K328	0490-1897		RELAY-REED 2A 1A 300VDC 5VDC-COIL	04501	3500-0113
L101-L102	9170-1663	3	CORE-SHIELDING BEAD	11702	FBM4532HM132
L104	9170-1584	12	CORE-SHLD BEAD	09808	25Z0805-0SR
L109-L115	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L150-L153	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L300	9170-1663		CORE-SHIELDING BEAD	11702	FBM4532HM132
L301-L302	9140-1638	2	INDUCTOR 10UH +-10% -10% 2.7W-MMX3.4LG-MM	06352	NLC322522T-100K
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
Q101	1855-1101	1	TRANSISTOR	02037	MMDFP2P02E
Q201-Q218	1854-1053	19	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q220	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
R102-R103	0699-3034	6	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R105	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R106-R109	0699-3970	5	RES 10K 1% .063W	06337	232270461003
R110-R112	0699-3974	3	Resistor 14.7K 1% 0603 50V .063W TC=200	06337	9C0603A1472FL
R113	0699-3970		RES 10K 1% .063W	06337	232270461003

Chapter 7 Replaceable Parts
HP 34902A 16-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R114	0699-2973	6	RES 215, FIXED THIN FILM	06337	9C08052A2150FKR
R115	0699-3067	1	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R117-R135	0699-3051	21	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R136-R138	0699-3947	10	RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R140	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R141-R143	0699-3947		RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R148	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	06337	9C08052A1004FKR
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R150-R151	0699-2973		RES 215, FIXED THIN FILM	06337	9C08052A2150FKR
R155-R158	0699-3947		RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R160-R162	0699-2973		RES 215, FIXED THIN FILM	06337	9C08052A2150FKR
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R170-R177	0699-3963	8	RESISTOR 4.64K 1% 0603 50V .063W TC=200	06337	9C0603A4641FL
R182-R183	0699-3932	4	RESISTOR 215 +-1% .063W TKF TC=0+-200	06337	9C0603A2150FL
R185-R186	0699-3932		RESISTOR 215 +-1% .063W TKF TC=0+-200	06337	9C0603A2150FL
R401-R404	0699-4867	4	RESISTOR 10 1% 12181.0w tc=0+-100	06337	23227351001
U101	34902-88821	1	PROGRAM PART	02632	34902-88821
U102-U104	1820-5752	3	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U150	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U151-U152	1821-2382	2	IC-DS1620S	12186	DS1620S
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
HP 34903A 20-Channel Actuator Rev B

HP 34903A 20-Channel Actuator Rev B

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C104	0160-7798	5	CAP 0.1UF +-10% 50V CER X7R	06352	C2012X7R1H104K
C107	0160-5947	1	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C110	0160-7798		CAP 0.1UF +-10% 50V CER X7R	06352	C2012X7R1H104K
C116-C118	0160-5947	3	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C121-C127	0160-5967		CAP-FXD 100pF +-5% 50 V CER COG	06352	C2012COG1H101J
C140	0160-7798		CAP 0.1UF +-10% 50V CER X7R	06352	C2012X7R1H104K
C141	0160-5945	8	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C150	0180-4545	1	CAP-FXD 4.7uF +-20% 20 V TA	12340	T491B475M020AS
C201-C207	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
CR101	1906-0395	3	DIODE-DUAL 75V TO-253	02910	BAS28
CR102	1906-0395	20	DIODE-DUAL 75V TO-253	02910	BAS28
CR103	1902-1544	1	DIODE-ZNR 10V 5% TO-236 (SOT-23) PD=.35W	02910	BZX84C10
CR201-CR220	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR221-CR222	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
CR224-CR225	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J301-J305	0360-2624	5	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
K208	0490-1896	20	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K301-K320	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L105	9170-1584	7	CORE-SHLD BEAD	09808	25Z0805-0SR
L109-L111	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
Q101	1855-1101	1	TRANSISTOR-MOSFET DUAL P-CHAN E-MODE SI	02037	MMDF2P02E
Q201	1854-1053	14	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q202-Q203	1853-0525	14	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q204	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q205	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q206-Q207	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q208-Q209	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q210	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q211	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q212-Q213	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q214	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q215	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q216-Q217	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907

Chapter 7 Replaceable Parts
HP 34903A 20-Channel Actuator Rev B

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q218	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q219	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q220-Q221	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q222-Q223	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q224	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q225	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q226-Q227	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q228	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
R102-R103	0699-3034	9	RESISTOR 1K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1001
R105	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1001
R106-R109	0699-3051	35	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R110-R112	0699-3067	3	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1472
R113	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R114	0699-2973	6	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R115	0699-3067		RESISTOR 14.7K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1472
R116-R118	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R120-R121	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R122-R127	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1001
R140	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1004
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1004
R170-R177	0699-3044	8	RESISTOR 4.64K +-1% .1W TKF TC=0+-100	06337	9C08052A4641FKR
R201-R228	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U101	34903-88801	1	PROGMD 1821-1876 MCU N87C52	02632	34903-88801
U102-U104	1820-5752	3	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U150	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
HP 34904A 4x8 Matrix

HP 34904A 4x8 Matrix

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C140	0160-7798	1	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C151	0160-5947	1	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C154-C157	0160-5945	12	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C158	0180-4545	1	CAP-FXD 4.7uF +-20% 20 V TA	12340	T491B475M020AS
C164-C166	0160-5967	2	CF 100PF 5% 0805	03292	0160-5967
C201-C207	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
CR101-CR109	1906-0291	33	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR110-CR111	1906-0395	3	DIODE-DUAL 75V TO-253	02910	BAS28
CR201-CR208	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR301-CR308	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR401-CR408	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR409	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J102-J107	0360-2623	6	CONN TERMNAL BK RA FEM 4 PIN	13389	M1.040.0001.8
K101-K108	0490-1896	32	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K201-K208	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K301-K308	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K401-K408	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L101-L102	9140-1782	2	INDUCTOR 4.7uH +10% -10%	06352	NLC565050T-4R7K
L105-L109	9170-1584	5	CORE-SHLD BEAD	09808	25Z0805-0SR
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
Q101	1855-1101	1	TRANSISTOR	02037	MMDF2P02E
Q111	1853-0525	12	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q113	1854-1053	12	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q121	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q123	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q131	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q133	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q141	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q143	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q211	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q213	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q221	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q223	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q231	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907

Chapter 7 Replaceable Parts
HP 34904A 4x8 Matrix

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q233	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q241	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q243	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q251	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q253	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q261	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q263	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q271	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q273	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q281	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q283	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
R111	0699-3051	32	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R113	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R121	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R123	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R131	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R133	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R141	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R143	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R147	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3053	1	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R151-R152	0699-3034	6	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R154	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R155	0699-3061	1	RESISTOR 261 +-1% .1W TKF TC=0+-100	06337	9C08052A2610FKR
R156-R158	0699-3067	3	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R160-R163	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R164-R165	0699-2973	2	RES 215, FIXED THIN FILM	06337	9C08052A2150FKR
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R211	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R213	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R221	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R223	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R231	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R233	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R241	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R243	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R251	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R253	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R261	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR

Chapter 7 Replaceable Parts
HP 34904A 4x8 Matrix

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R263	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R271	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R273	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R281	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R283-R284	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R287	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U101	34903-88801	1	PROGMD 1821-1876 MCU N87C52	02632	34903-88801
U102-U103	1820-5752	2	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U111	1818-6821	1	FRAM SERIAL 4K FM24C04-S	14543	FM24C04-S
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
HP 34905A/34906A RF Multiplexer

HP 34905A/34906A RF Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C103	0160-5945	9	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C111	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C140	0160-7798	1	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C151	0160-5947	1	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C158	0180-4545	1	CAP-FXD 4.7uF +20% 20 V TA	12340	T491B475M020AS
C164-C165	0160-5967	2	CF 100PF 5% 0805	03292	0160-5967
C201-C204	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
CR102	1906-0291	1	DIODE-DUAL 70V 100MA T0-236AA	02910	BAV99
CR170	1906-0395	1	DIODE-DUAL 75V T0-253	02910	BAS28
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
K101-K103	0490-1671	6	RELAY, RG1ET-L-3V	01850	RG1ET-L-3V-H14
K201-K203	0490-1671		RELAY, RG1ET-L-3V	01850	RG1ET-L-3V-H14
L105-L109	9170-1584	5	CORE-SHLD BEAD	09808	25Z0805-0SR
L170-L171	9140-1782	2	INDUCTOR 4.7uH +10% -10%	06352	NLC565050T-4R7K
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
P1-P10	1250-1377	10	CONNECTOR-RF SMB PLUG PC-W/O-STDF 50-OHM	03621	5164-5003-09
Q101	1854-1053	12	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q102	1853-0525	36	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q103	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q104	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q105	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q106	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q107	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q108	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q109	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q110	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q111	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q112	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q170	1855-1101	1	TRANSISTOR-MOSFET DUAL P-CHAN E-MODE SI	02037	MMDFP020E
Q201	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q202	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q203	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q204	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q205	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q206	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q207	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q208	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q209	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q210	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907

Chapter 7 Replaceable Parts
HP 34905A/34906A RF Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q211	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q212	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q231-Q254	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
R27	0699-3034		RESISTOR 1K +1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R101-R112	0699-3040	24	RESISTOR 3.16K +-1% .1W TKF TC=0+-100	02995	9C08052A3161FKR
R140	0699-3051	7	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3053	1	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R151-R152	0699-3034	7	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R154	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R155	0699-3061	1	RESISTOR 261 +-1% .1W TKF TC=0+-100	06337	9C08052A2610FKR
R156-R158	0699-3067	3	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R159-R163	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R164-R165	0699-2973	2	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R201-R212	0699-3040		RESISTOR 3.16K +-1% .1W TKF TC=0+-100	02995	9C08052A3161FKR
SH101	34905-60601	4	SHIELD-RF	01642	34905-60601
SH103	34905-60601		SHIELD-RF	01642	34905-60601
SH201	34905-60601		SHIELD-RF	01642	34905-60601
SH203	34905-60601		SHIELD-RF	01642	34905-60601
U101	34903-88801	1	PROGMD 1821-1876 MCU N87C52	02632	34903-88801
U102-U103	1820-5752	2	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U111	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07
For HP 34906A 75 Ω RF Multiplexer					
K101-K103	0490-1672	6	RELAY, 1C 3VDC-COIL 1A 24 VDC	01850	RG1E-L-3V-H13
K201-K203	0490-1672		RELAY, 1C 3VDC-COIL 1A 24 VDC	01850	RG1E-L-3V-H13
P1-P10	1250-2339	10	CONNECTOR-RF SMB-PLUG PC-W/O-STDF 75-OHM	03621	131-8701-301

Chapter 7 Replaceable Parts
HP 34907A Multifunction Module

HP 34907A Multifunction Module

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C102	0160-7798	17	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C103	0160-5945	9	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C104-C105	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C106-C108	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C110-C112	0160-5967	9	CAP-FXD 100pF +5% 50 V CER C0G	03292	0160-5967
C120	0160-5947	4	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C140	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C150	0180-4545	1	CAP-FXD 4.7uF +20% 20 V TA	12340	T491B475M020AS
C203	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C204	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C205	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C206-C207	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C208	0180-4287	5	CAP-FXD 10uF +20% 35 V TA	05524	293D106X0035D2W
C211-C214	0160-5967		CAP-FXD 100pF +5% 50 V CER C0G	03292	0160-5967
C301	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C302	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C401	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C402	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C502-C505	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C506	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C507-C508	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C510	0180-4116	1	CAP-FXD 22uF 20 V TA	00039	NRD226M20R12
C511	0160-6218	1	CAP-FXD 4700pF 50 V	12473	0160-6218
C512	0160-5944	1	CAP-FXD 0.047uF 50 V	12473	0160-5944
C513-C514	0180-4287		CAP-FXD 10uF +20% 35 V TA	05524	293D106X0035D2W
C515-C516	0180-3751	2	CAP-FXD 1uF +20% 35 V TA	00039	NRS105M35R8
C520	0180-4287		CAP-FXD 10uF +20% 35 V TA	05524	293D106X0035D2W
C521	0180-3744	1	TANT SMD 4.7 20%	00039	NRS475M10R8
C522	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C523	0180-4228	1	CAP-FXD 47uF 10 V TA	05524	293D476X00101D2W
C524	0180-4287		CAP-FXD 10uF +20% 35 V TA	05524	293D106X0035D2W
C531	0160-5967		CAP-FXD 100pF +5% 50 V CER C0G	03292	0160-5967
C532	0160-5947		CAP-FXD 1000pF 50 V	02010	08055C102KATA
C533	0160-5967		CAP-FXD 100pF +5% 50 V CER C0G	03292	0160-5967
C534	0160-5947		CAP-FXD 1000pF 50 V	02010	08055C102KATA
C550-C551	0160-7733	2	CAP-FXD 100pF +1% 50 V CER C0G	12340	C0805C101F5GAC
C552	0160-5947		CAP-FXD 1000pF 50 V	02010	08055C102KATA
CR101-CR106	1906-0358	22	DIODE-DUAL 100V 100MA T0-236AB (SOT-23)	03406	MMBD1203-HIGH
CR110	1906-0291	4	DIODE-DUAL 70V 100MA T0-236AA	02910	BAV99

**Chapter 7 Replaceable Parts
HP 34907A Multifunction Module**

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
CR301-CR308	1906-0358		DIODE-DUAL 100V 100MA TO-236AB (SOT-23)	03406	MMBD1203-HIGH
CR401-CR408	1906-0358		DIODE-DUAL 100V 100MA TO-236AB (SOT-23)	03406	MMBD1203-HIGH
CR501-CR504	1901-1386	4	DIO SI PN SOT23 100V 750MA BAS78B	06121	BAS78B
CR505-CR506	1902-1643	2	DIODE-ZNR 15V PD=1.5W IR=1UA	02037	1SMB5929B
CR507	1901-1402	1	DIO SCH PWR SOD123 30V 500MA 10PE BAT65	06121	BAT65
CR510-CR511	1901-1332	2	DIODE-UNMOUNTED CHIP	03038	10BQ040
CR520-CR521	1906-0291		DIODE-DUAL 70V 100MA T0-236AA	02910	BAV99
CR530	1901-1348	1	DIO TVS UNIDIR SMB 24V 600WP SMBJ24A	03287	SMBJ24A
CR531	1906-0291		DIODE-DUAL 70V 100MA T0-236AA	02910	BAV99
FB501-FB506	9170-1584	8	CORE-SHLD BEAD	09808	25Z0805-0SR
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
L105	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L109	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L201-L202	9140-1782	2	INDUCTOR 4.7uH +10% -10%	06352	NLC565050T-4R7K
L501-L502	9140-1638	2	INDUCTOR 10UH +10% -10% 2.7W-MMX3.4LG-MM	06352	NLC322522T-100K
L510	9140-2152	1	L SMT 22uH 20% 1.32A	05524	LPE-4841 220UH +/-20% B
L515-L516	9140-1238	2	INDUCTOR 10UH +5% 2.8W-MMX3.4LG-MM Q=30	02366	KL32TE100J
MAL510	34907-00601	1	SHIELD	02631	34907-00601
MAP102	1258-0209	1	JUMPER - REMOVABLE, TWO POSITION	01380	531220-2
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
P101	0360-2623	2	CONN TERMNAL BK RA FEM 4 PIN	13389	M1.040.0001.8
P102	1251-4670	1	CONN-POST TYPE .100-PIN-SPCG 3-CONT	04726	2403-6112TB
P301	0360-2624	2	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
P401	0360-2624		CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
P501	0360-2623		CONN TERMNAL BK RA FEM 4 PIN	13389	M1.040.0001.8
Q301-Q308	1855-0800	16	TRANSISTOR MOSFET N-CHAN E-MODE TO-252AA	02037	MTD3055EL
Q401-Q408	1855-0800		TRANSISTOR MOSFET N-CHAN E-MODE TO-252AA	02037	MTD3055EL
R101-R102	0699-3034	8	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R104	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R105	0699-3053	4	RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R108	0699-3053		RESISTOR 100K +-1% .1W TKF TC=0+-100	02995	9C08052A1003FKR
R109	0699-3051	4	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R110-R111	0699-2973	10	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR

Chapter 7 Replaceable Parts
HP 34907A Multifunction Module

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
R112	0699-3053		RESISTOR 100K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1003FKR
R113	0699-3070	1	RESISTOR 26.1K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A2612FKR
R114	0699-3044	3	RESISTOR 4.64K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A4641FKR
R115	0699-3052	5	RESISTOR 12.1K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1212FKR
R116	0699-2997	1	RESISTOR 133K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1333FKR
R117	0699-3052		RESISTOR 12.1K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1212FKR
R118	0699-3044		RESISTOR 4.64K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A4641FKR
R119	0699-2986	1	RESISTOR 21.5K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A2152FKR
R120-R123	0699-1319	16	RESISTOR 12.1K $\pm 1\%$.125W TKF TC=0 \pm 100	04935	9C12063AFKR
R124	0699-3008	4	RESISTOR 511K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A5113FKR
R125-R128	0699-1319		RESISTOR 12.1K $\pm 1\%$.125W TKF TC=0 \pm 100	04935	9C12063AFKR
R129	0699-3008		RESISTOR 511K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A5113FKR
R130-R133	0699-1319		RESISTOR 12.1K $\pm 1\%$.125W TKF TC=0 \pm 100	04935	9C12063AFKR
R134-R135	0699-3008		RESISTOR 511K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A5113FKR
R140	0699-3052		RESISTOR 12.1K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1212FKR
R141	0699-3049	1	RESISTOR 8.25K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A8251FKR
R148	0699-3053		RESISTOR 100K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1003FKR
R151-R153	0699-2643	3	RESISTOR 0 $\pm 5\%$.1W TKF TC=0 \pm 300	06337	9C08052A0R00JL
R166-R168	0699-3034		RESISTOR 1K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1001FKR
R205	0699-3051		RESISTOR 10K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1002FKR
R211-R214	0699-2973		RESISTOR 215 $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A2150FKR
R215-R216	0699-3051		RESISTOR 10K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1002FKR
R301	0699-3047	1	RESISTOR 6.81K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A6811FKR
R302	0699-3045	1	RESISTOR 5.11K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A5111FKR
R501	0699-3602	2	RESISTOR 12.4K $\pm 0.1\%$.125W TF TC=0 \pm 25	06337	9C12063A1242BE
R502	0699-2838	2	RESISTOR 40K $\pm 0.1\%$.125W TF TC=0 \pm 25	06337	9C12063A4002BE
R503	0699-3602		RESISTOR 12.4K $\pm 0.1\%$.125W TF TC=0 \pm 25	06337	9C12063A1242BE
R504	0699-2838		RESISTOR 40K $\pm 0.1\%$.125W TF TC=0 \pm 25	06337	9C12063A4002BE
R505-R506	0699-3052		RESISTOR 12.1K $\pm 1\%$.1W TKF TC=0 \pm 100	02995	9C08052A1212FKR
R510	0699-3036	1	RESISTOR 1.96K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1961FKR
R511	0699-3046	1	RESISTOR 6.19K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A6191FKR
R512	0699-2962	1	RESISTOR 68.1K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A6812FKR
R513	0699-3044		RESISTOR 4.64K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A4641FKR
R514	0699-3034		RESISTOR 1K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1001FKR
R518	0699-3034		RESISTOR 1K $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A1001FKR
R531-R534	0699-2973		RESISTOR 215 $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A2150FKR
R550-R551	0699-3832	2	RESISTOR 51.1 $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A511R1FK
R552	0699-3061	1	RESISTOR 261 $\pm 1\%$.1W TKF TC=0 \pm 100	06337	9C08052A2610FKR
R553-R556	0699-1319		RESISTOR 12.1K $\pm 1\%$.125W TKF TC=0 \pm 100	04935	9C12063AFKR
RP101-RP105	1810-1580	12	RESISTOR; CARBON FILM;NTWRK	00746	MNR34K5AWJ103
RP201-RP204	1810-1831	4	NETWORK-RES 620 X 4 5% 1206 .125W 200V	09891	CN2B4TE621J

Chapter 7 Replaceable Parts
HP 34907A Multifunction Module

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
RP301-RP304	1810-1660	4	NETWORK-RES 3.3KX4 5% 1206 .125W 200W	09891	CN2B4332J
RP305-RP306	1810-1521	4	NETWORK-RES 100K X 4 5% 1206 .125W 200V	09891	CN2B4104J
RP307-RP308	1810-1580		RESISTOR; CARBON FILM;NTWRK	00746	MNR34K5AWJ103
RP401-RP402	1810-1660		NETWORK-RES 3.3KX4 5% 1206 .125W 200W	09891	CN2B4332J
RP403-RP404	1810-1580		RESISTOR; CARBON FILM;NTWRK	00746	MNR34K5AWJ103
RP405-RP406	1810-1521		NETWORK-RES 100K X 4 5% 1206 .125W 200V	09891	CN2B4104J
RP407-RP408	1810-1580		RESISTOR; CARBON FILM;NTWRK	00746	MNR34K5AWJ103
U101	34907-88811	1	PROGRAM PART	02632	34907-88811
U102	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U103	1820-7312	1	IC SCHMITT-TRIG CMOS/ACT INV HEX	02037	MC74ACT14DR2
U104	1820-4220	1	IC GATE CMOS/HC OR QUAD 2-INP	02910	74HC32D
U105-U106	1820-5752	6	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U107	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U108	1826-2116	1	IC OP AMP LP DUAL 8 PIN PLSTC-SOIC	02037	MC34182D
U109	1826-1594	1	IC COMPARATOR GP SINGLE 8 PIN PLSTC-SOIC	04078	LM311D
U110	1820-5804	1	IC SHF-RGTR CMOS/HC SYNC/ASYNC	02037	MC74HC165D
U111	1820-4938	1	IC GATE CMOS/HC EXCL-OR QUAD 2-INP	02910	74HC86D
U201-U204	1820-5752		IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U205-U206	1820-4216	2	IC DRVR CMOS/HC BUS OCTL	02910	74HC240D
U301-U302	1826-1225	4	IC COMPARATOR LP QUAD 14 PIN PLSTC-SOIC	03406	LP339M
U401-U402	1826-1225		IC COMPARATOR LP QUAD 14 PIN PLSTC-SOIC	03406	LP339M
U502	1826-3088	1	IC PWR MGT-V-REG-ADJ-NEG -5.25/-4.75V 8	11302	MAX735CSA
U503-U504	1826-2793	2	D/A 16-BIT 16-P-SOIC BICMOS	03285	AD1851R
U505-U506	1826-2819	2	IC OP AMP PRCN SINGLE 8 PIN PLSTC-SOIC	03285	OP177GS
U510	1826-3193	1	IC PWR MGT-V-REG-SWG 8 PINS P-SOIC PKG	10858	LT1372CS8
VR101-VR104	1901-1410	4	DIO TVS BIDIR SMB 600WP 110V SMBJ110C	03287	SMBJ110C
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
HP 34908A 40-Channel Multiplexer

HP 34908A 40-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C106	0160-7798	9	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C107	0160-7708	1	CAP-FXD 1000pF +-5% 50 V CER COG	12340	C0805C102J5GAC
C109	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C110	0160-7828	1	CAP .1UF 16V 10% X7R	02010	0603C104KAT
C119-C123	0160-5947	5	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C125-C128	0160-7845	4	CAP FXD 180PF +-5% 50 V CER COG	12340	C0603C181J5GAC
C130-C135	0160-7751	6	CAP-FXD 0.01uF +-10% 50 V CER X7R	12340	C0603C103K5RAC
C140-C141	0160-5945	12	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C145	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C150	0180-4545	1	CAP-FXD 4.7uF +-20% 20 V TA	12340	T491B475M020AS
C151-C152	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C201-C208	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C209	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
CR102	1906-0395	5	DIODE-DUAL 75V TO-253	02910	BAS28
CR103-CR106	1902-1574	4	DIODE-ZNR 6.8V 6% TO-236 (SOT-23)	02910	BZX84C6V8
CR107	1906-0291	22	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR201-CR220	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR221-CR222	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
CR223	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR224-CR225	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J102-J104	0360-2624	4	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
J106	0360-2624		CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
K401-K420	0490-1896	20	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K421	0490-1895	1	RLY-2C 2A 220V 60WATT 4.5V COIL	12921	G6S-2-DC4.5
K422	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L101-L103	9170-1663	4	CORE-SHIELDING BEAD	11702	FBM4532HM132
L105	9170-1584	12	CORE-SHLD BEAD	09808	25Z0805-0SR
L109-L115	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L150-L153	9170-1584		CORE-SHLD BEAD	09808	25Z0805-0SR
L400	9170-1663		CORE-SHIELDING BEAD	11702	FBM4532HM132
MP1	34901-60001		KIT, MODULE COVER, CASE	02362	34901-60001
Q101	1855-1101	1	TRANSISTOR-MOSFET DUAL P-CHAN E-MODE SI	02037	MMDF2P02E
Q201	1854-1053	17	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q202-Q203	1853-0525	16	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907

Chapter 7 Replaceable Parts
HP 34908A 40-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q204	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q205	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q206-Q207	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q208-Q209	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q210	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q211	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q212-Q213	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q214	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q215	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q216-Q217	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q218	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q219	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q220-Q221	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q222-Q223	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q224	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q225	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q226-Q227	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q228	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q229	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q230	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q231	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q232	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q233	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
R102-R105	0699-3034	12	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R106-R109	0699-3051	40	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R110-R112	0699-3067	5	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R113	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R114-R115	0699-3067		RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R117-R120	0699-2973	4	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R147	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	06337	9C08052A1004FKR
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R150-R153	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R154-R157	0699-3947	4	RESISTOR 1K +-1% .063W TKF TC=0+-200	06337	9C0603A1001FL
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R170-R180	0699-3044	11	RESISTOR 4.64K +-1% .1W TKF TC=0+-100	06337	9C08052A4641FKR
R181	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R182-R186	0699-3932	4	RESISTOR 215 +-1% .063W TKF TC=0+-200	06337	9C0603A2150FL
R201-R233	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U101	34901-88811	1	PRGM'D 1821-1876	02632	34901-88811

Chapter 7 Replaceable Parts
HP 34908A 40-Channel Multiplexer

Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
U102-U105	1820-5752	4	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U109	1820-5941	1	IC DCDR-DEMUXR CMOS/ACT BIN 8-TO-1-LINE	03406	74ACT138SC
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U150	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
U151-U152	1821-2382	2	IC-INTERFACE MISC BIPOLAR 9-BIT	12186	DS1620S
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Chapter 7 Replaceable Parts
Manufacturer's List

Manufacturer's List

Mfr Code	Mfr Name	City	State	Country
00039	NEC ELECTRONICS INC	MTN VIEW	CA	US
00746	ROHM CORP	KYOTO 615		JP
00830	KYOCERA AMERICA, INC	SAN DIEGO	CA	US
01380	AMP INC	HARRISBURG	PA	US
01542	HP DIV 01 SAN JOSE COMPONENTS	SAN JOSE	CA	US
01642	SONS TOOL INC	WOODVILLE	WI	US
01698	TEXAS INSTRUMENTS INC	DALLAS	TX	US
01850	AROMAT CORP	MOUNTAINSIDE	NJ	US
02010	AVX CORP	GREAT NECK	NY	US
02037	MOTOROLA INC	ROSELLE	IL	US
02194	ROBINSON NUGENT INC	NEW ALBANY	IN	US
02237	FAIRCHILD SEMICONDUCTOR	SOUTH PORTLAND	ME	US
02361	HP DIV 09 LID SHEET METAL 02	LOVELAND	CO	US
02362	HP DIV 09 LID COMPONENTS	LOVELAND	CO	US
02499	INTERNATIONAL RESISTIVE CO.	BOONE	NC	US
02883	TEMIC/SILICONIX INC	SANTA CLARA	CA	US
02910	PHILIPS SEMICONDUCTORS	EINDHOVEN		NL
03038	INTL RECTIFIER CORP	LOS ANGELES	CA	US
03285	ANALOG DEVICES INC	NORWOOD	MA	US
03287	GENERAL SEMICONDUCTOR IND INC	TEMPE	AZ	US
03292	CORNING GLASS WORKS	CORNING	NY	US
03406	NATIONAL SEMICONDUCTOR CORP	SANTA CLARA	CA	US
03418	MOLEX INC	LISLE	IL	US
03677	AMERICAN MICRO SYSTEMS INC	SANTA CLARA	CA	US
03744	BOURNS NETWORKS INC	RIVERSIDE	CA	US
03811	INTEL CORP	SANTA CLARA	CA	US
03827	FAIR RITE PRODUCTS CORP	WALLKILL	NY	US
04078	SGS-THOMSON MICROELECTRONICS INC	PHOENIX	AZ	US
04501	COTO WABASH	PROVIDENCE	RI	US
04504	GENERAL INSTRUMENT CORP	CHICAGO	IL	US
04670	JOHNSON COMPONENTS INC	WASECA	MN	US
04726	3M CO	ST PAUL	MN	US

Chapter 7 Replaceable Parts
Manufacturer's List

Mfr Code	Mfr Name	City	State	Country
04733	BELL INDUSTRIES INC MILLER JW DIV	GARDENA	CA	US
05176	AMERICAN SHIZUKI CORP	CANOGA PARK	CA	US
05524	VISHAY INTERTECHNOLOGY INC	MALVERN	PA	US
05525	ELCO CORP	NEWPORT BEACH	CA	US
05535	KEYSTONE ELECTRONICS CORP	NEW YORK	NY	US
05951	WICKMANN-WERKE A G	WITTEN-ANNEN		DE
06121	SIEMENS AG	MUNICH		DE
06337	PHILIPS ELECTRONICS NV	EINDHOVEN		NL
06352	TDK CORPORATION OF AMERICA	SKOKIE	IL	US
06360	NIPPON CHEMI-CON CORP	OHME-SHI TOKYO		JP
06916	SONY CORP	TOYKO		JP
07179	AAVID THERMAL TECHNOLOGY INC	LACONIA	NH	US
08709	MATSUSHITA ELECTRIC CORPORATION OF	SECAUCUS	NJ	US
09235	FOX ELECTRONICS	FT MEYERS	FL	US
09454	PRECISION RESISTIVE PRODS INC	MEDIAPOLIS	IA	US
09808	STEWART INC	CHATTANOOGA	TN	US
09891	KOA CORPORATION	INA-SHI NAGANO-KEN		JP
09939	MURATA ELECTRONICS NORTH AMERICA, INC.	LONG BEACH	CA	US
10421	EPSON AMERICA INC	TORRENCE	CA	US
10858	LINEAR TECHNOLOGY CORP	MILPITAS	CA	US
11302	MAXIM INTEGRATED PRODUCTS	SUNNYVALE	CA	US
11484	JOSLYN ELECTRONIC SYSTEMS DIV	GOLETA	CA	US
11702	TAIYO YUDEN CO LTD	TOKYO 110		JP
11908	NORITAKE CO LTD	NISHI-KU - NAGOYA		JP
12125	SAMSUNG SEMICONDUCTOR INC	SANTA CLARA	CA	US
12186	DALLAS SEMICONDUCTOR CORP	DALLAS	TX	US
12340	KEMET ELECTRONICS CORPORATION	GREENVILLE	SC	US
12768	SEIKO EPSON CORP	NAJANO-KEN TOKYO		JP
12921	OMRON JAPAN	KYOTO		JP
13389	WIELAND INC	ROCHELLE	NY	US
14543	RAMTRON	COLORADO SPRINGS	CO	US

 Backdating

Backdating

This chapter contains information necessary to adapt this manual to instruments not directly covered by the current content.

The HP 34903A 20-Channel Actuator is the only revised module at the time of this printing. The original Rev A replaceable parts list is given below.

HP 34903A 20-Channel Actuator Rev A


Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
C101-C104	0160-7798	5	CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C107	0160-5947	1	CAP-FXD 1000pF 50 V	02010	08055C102KATA
C116-C118	0160-5967	3	CF 100PF 5% 0805	03292	0160-5967
C140	0160-7798		CAP 0.1UF 50V 10% X7R 0805	02010	08055C104KAT_A
C141	0160-5945	8	CAP-FXD 0.01uF 50 V	02010	08055C103KATA
C150	0180-4545	1	CAP-FXD 4.7uF +20% 20 V TA	12340	T491B475M020AS
C201-C207	0160-5945		CAP-FXD 0.01uF 50 V	02010	08055C103KATA
CR101	1906-0395	3	DIODE-DUAL 75V TO-253	02910	BAS28
CR102	1906-0291	20	DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR103	1902-1544	1	DIODE-ZNR 10V 5% TO-236 (SOT-23) PD=.35W	02910	BZX84C10
CR201-CR220	1906-0291		DIODE-DUAL 70V 100MA TO-236AA	02910	BAV99
CR221-CR222	1906-0395		DIODE-DUAL 75V TO-253	02910	BAS28
J101	1252-8024	1	CONN-POST TYPE .100-PIN-SPCG-MTG-END	05525	26-8477-048-002-025
J301-J305	0360-2624	5	CONN TERMINAL BK RA FEM 12PIN	13389	M1.040.0001.9
K208	0490-1896	20	RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
K301-K320	0490-1896		RLY-2C 2A 220V 60WATT 3V-COIL LATCHING	12921	G6SU-2-DC3
L101-L102	9140-1782	2	INDUCTOR 4.7uH +10% -10%	06352	NLC565050T-4R7K
L105-L111	9170-1584	7	CORE-SHLD BEAD	09808	25Z0805-OSR
Q101	1855-1101	1	TRANSISTOR-MOSFET DUAL P-CHAN E-MODE SI	02037	MMDF2P02E
Q201	1854-1053	14	TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q202-Q203	1853-0525	14	TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q204	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q205	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q206-Q207	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q208-Q209	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q210	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A


Reference Designator	HP Part Number	Qty	Part Description	Mfr Code	Mfr Part Number
Q211	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q212-Q213	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q214	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q215	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q216-Q217	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q218	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q219	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q220-Q221	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q222-Q223	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q224	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q225	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
Q226-Q227	1854-1053		TRANSISTOR NPN SI SOT-23 (TO-236AB)	12125	KST2222A
Q228	1853-0525		TRANSISTOR PNP SI TO-236AA PD=200MW	02237	MMBT2907
R101	0699-3061	1	RESISTOR 261 +-1% .1W TKF TC=0+-100	06337	9C08052A2610FKR
R102-R103	0699-3034	9	RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R105	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R106-R109	0699-3051	35	RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R110-R112	0699-3067	3	RESISTOR 14.7K +-1% .1W TKF TC=0+-100	06337	9C08052A1472FKR
R113	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R114	0699-2973	6	RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R116-R118	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R120-R121	0699-2973		RESISTOR 215 +-1% .1W TKF TC=0+-100	06337	9C08052A2150FKR
R122-R124	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R140	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R148	0699-3077	1	RESISTOR 1M +-1% .1W TKF TC=0+-100	00746	MCR10-F-X-1004
R149	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
R166-R168	0699-3034		RESISTOR 1K +-1% .1W TKF TC=0+-100	06337	9C08052A1001FKR
R170-R177	0699-3044	8	RESISTOR 4.64K +-1% .1W TKF TC=0+-100	06337	9C08052A4641FKR
R201-R228	0699-3051		RESISTOR 10K +-1% .1W TKF TC=0+-100	06337	9C08052A1002FKR
U101	34903-88801	1	PROGMD 1821-1876 MCU N87C52		
U102-U104	1820-5752	3	IC FF CMOS/HC D-TYPE POS-EDGE-TRIG COM	02910	74HC574D
U141	1821-0055	1	IC SCHMITT-TRIG CMOS/ACT NAND QUAD 2-INP	02037	MC74ACT132D
U150	1818-6821	1	FRAM SERIAL 4K FMZ4C04-S	14543	FM24C04-S
XU101	1200-1592		SOCKET-IC-PLCC 44-CONT SQUARE J-LEAD	01380	3-822275-1
Y101	0410-4009	1	CERO-RES 12MHZ +1-0.8%	00830	PBRC-12.0BRN07

Schematics and Diagrams

This chapter contains a block diagram, schematics, and component locator drawings for the instrument and all plug-in modules. The block diagram and schematics support the Theory of Operation in Chapter 5.


- HP 34970A System Block Diagram, *on page 205*
- A1 Component Locator, *on page 206*
- A1 Schematics, *start on page 208*
- A2 Component Locator, *on page 212*
- A2 Schematic, *on page 213*
- A3 Component Locator, *on page 214*
- A3 Schematic, *on page 215*
- A4 Component Locator, *on page 216*
- A4 Schematics, *start on page 218*
- HP 34901A 20-Channel Multiplexer Component Locator, *on page 222*
- HP 34901A 20-Channel Multiplexer Schematics, *start on page 223*
- HP 34902A 16-Channel Multiplexer Component Locator, *on page 228*
- HP 34902A 16-Channel Multiplexer Schematics, *start on page 229*
- HP 34903A 20-Channel Actuator Component Locator, *on page 233*
- HP 34903A 20-Channel Actuator Schematics, *start on page 234*
- HP 34904A 4x8 Matrix Component Locator, *on page 237*
- HP 34904A 4x8 Matrix Schematics, *start on page 238*
- HP 34905A/34906A RF Multiplexer Component Locator, *on page 241*
- HP 34905A/34906A RF Multiplexer Schematics, *start on page 242*
- HP 34907A Multifunction Module Component Locator, *on page 244*
- HP 34907A Multifunction Module Schematics, *start on page 245*
- HP 34908A 40-Channel Multiplexer Component Locator, *on page 250*
- HP 34908A 40-Channel Multiplexer Schematics, *start on page 251*


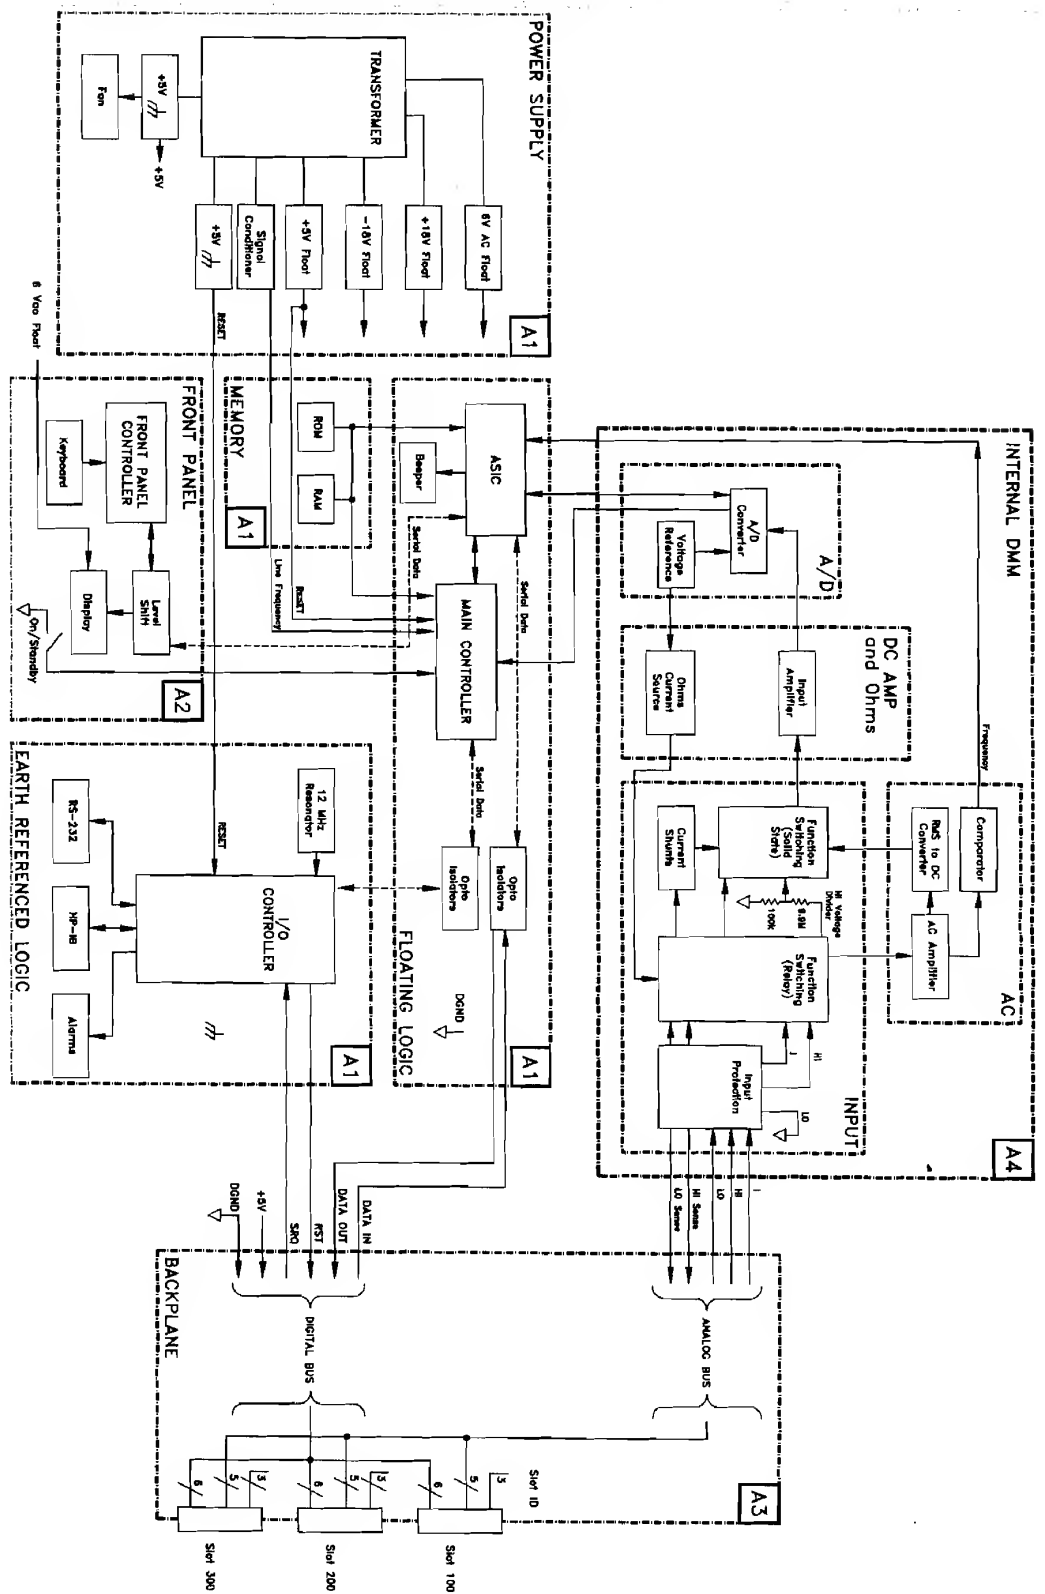


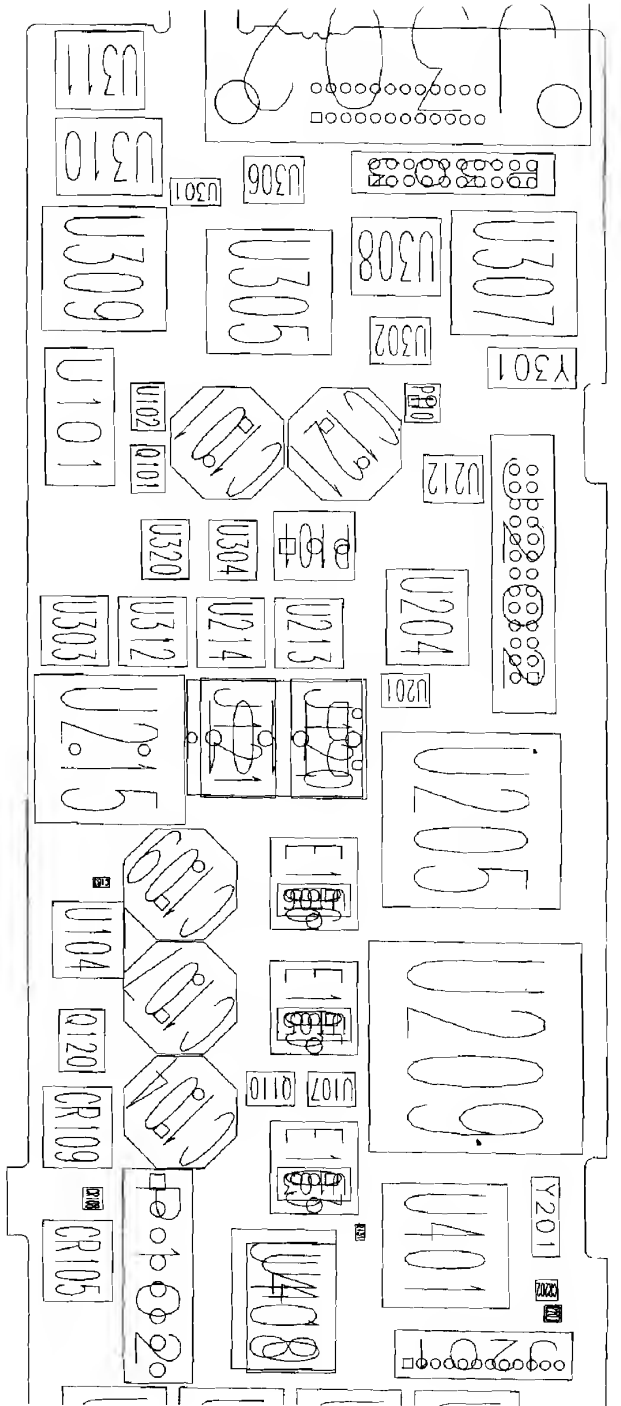


34970-66501 R


A1 Component Locator (Rev)
206

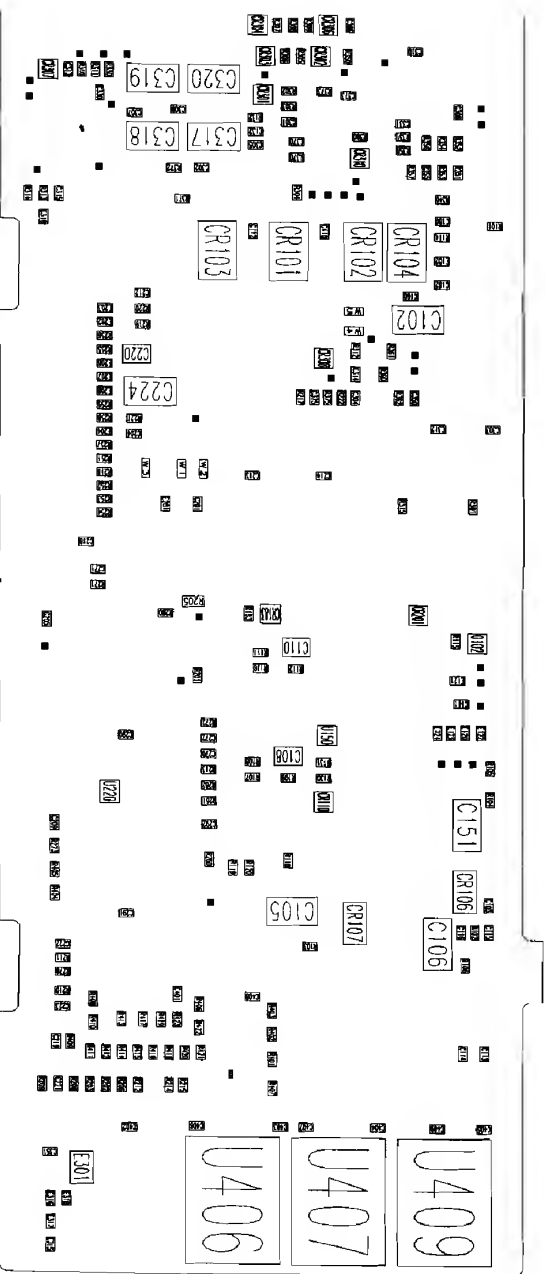


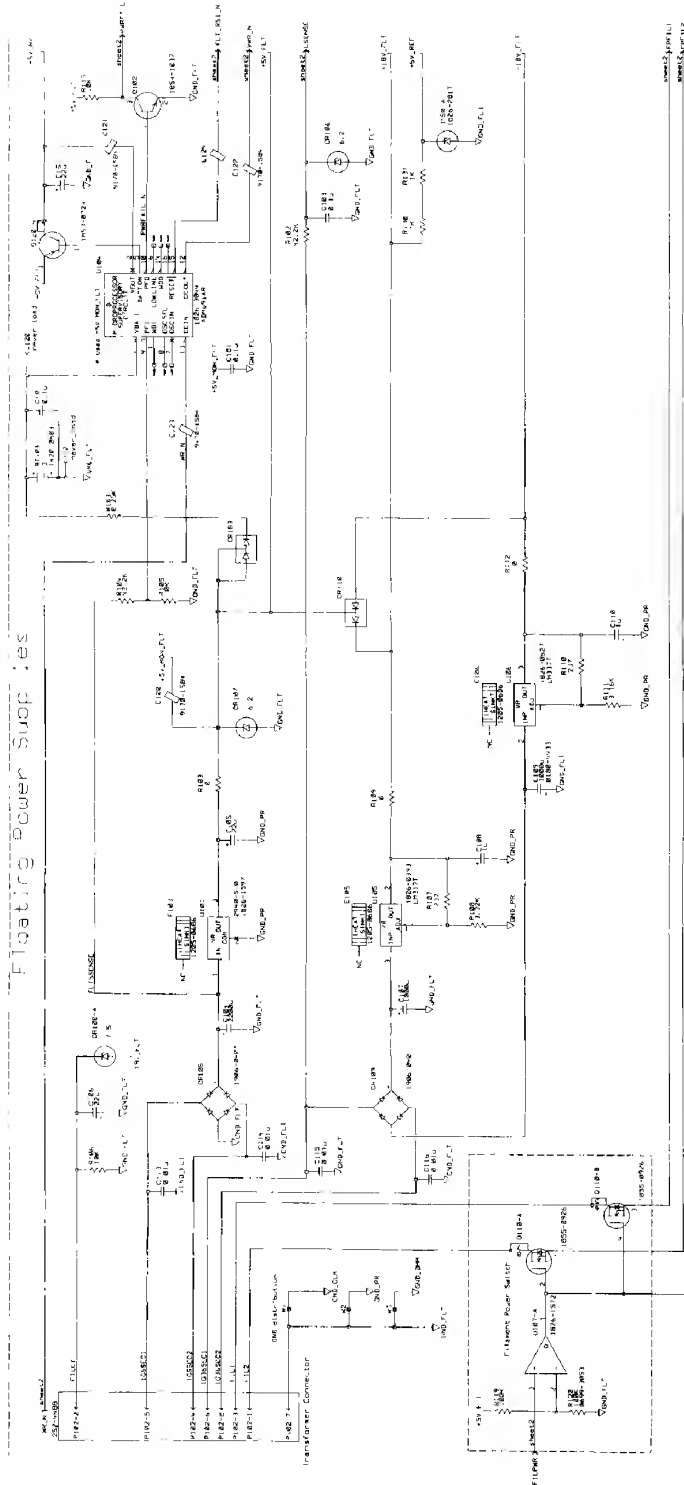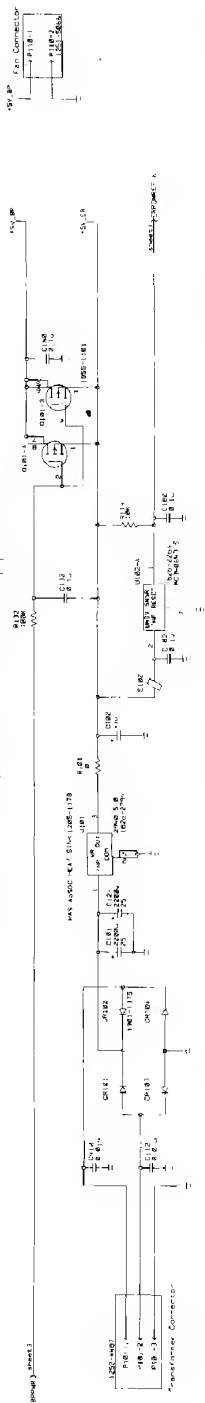

REV	DESCRIPTION	DATE
1	INITIAL DESIGN	11/11/11
2	REVISION	11/11/11



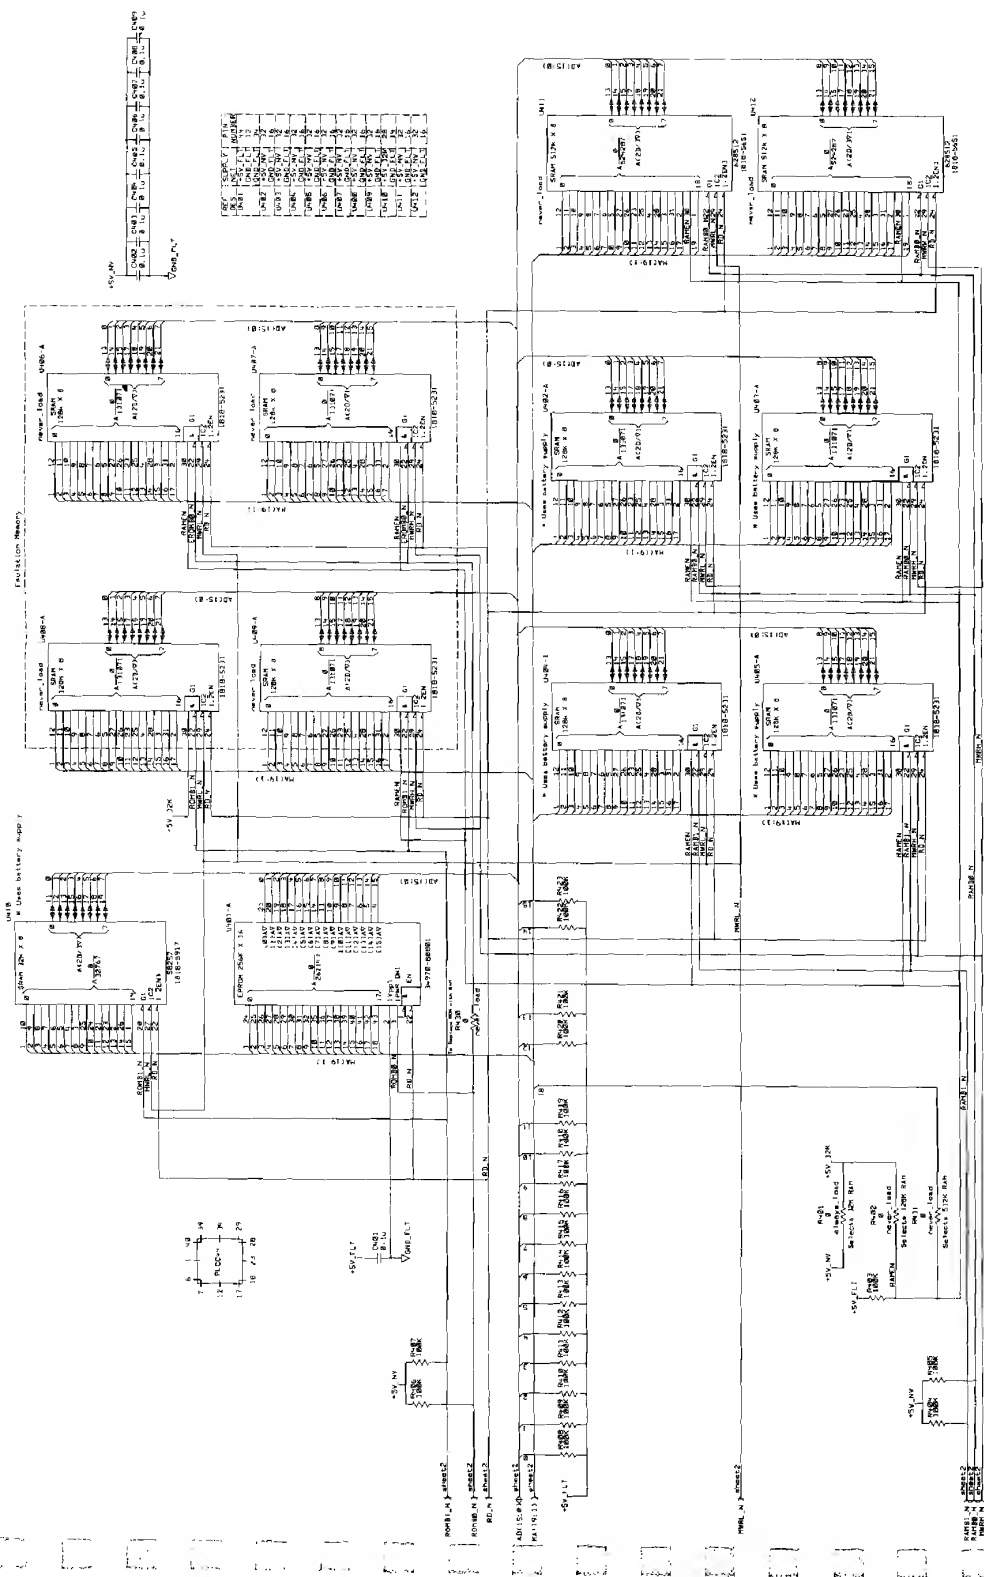

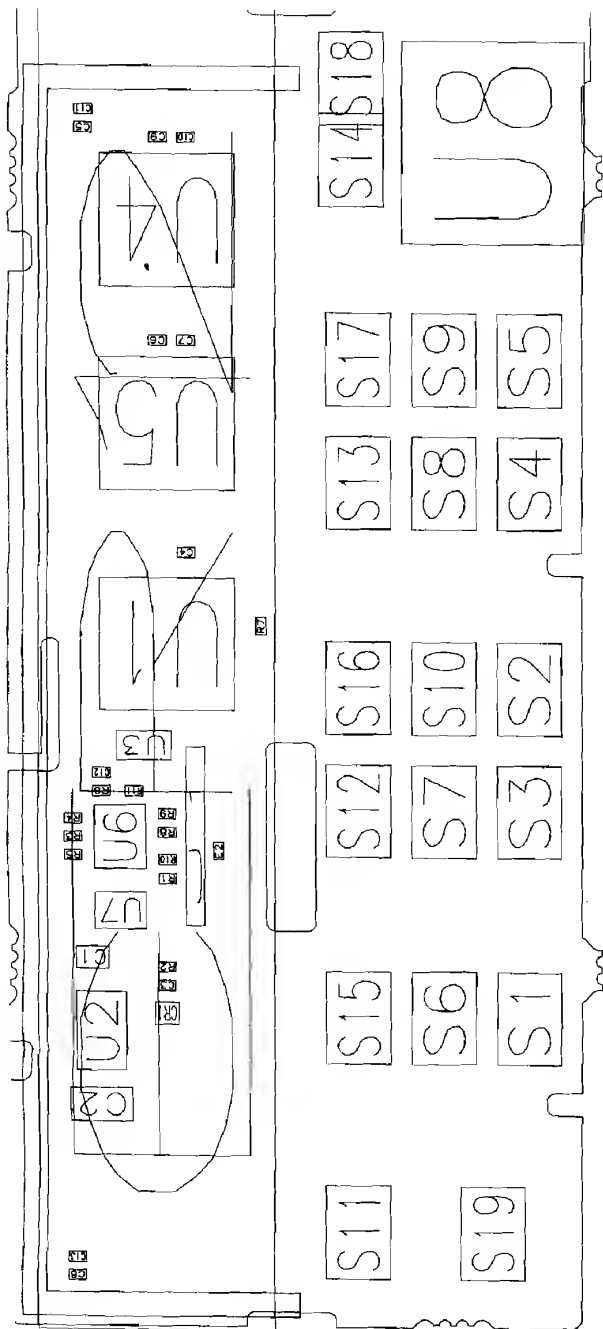

34970-66502 Rev 1
 AS Component Locator
 212

RV101

J1

R160

P101

E101

L102

RV102

P106

P105

P102

E102




R110

L101

C109
R101

P103

P104

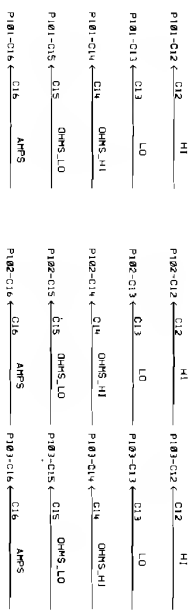

U308

P 1 0 0

CR302

U302

U303

U301

R

U403

C407

C401

C409

C402

CR403

W100

Q301

CR404

C408

U402

U420

U311

U309

C323

U103

R303

C305

Q104

U105

U304

C318

C321

CR306

CR304

CR401

CR402

C403

C404

L402

L401

C322

R442

CR103

U153

R127

Q153

Q152

U104

U106

U107

CR303

C349

U307

C330

U400

U411

U401

U310

C316

U306

U312

U305

CR203

U102

U101

R183

R173

L111

Q201


U201


R202

R201




C111







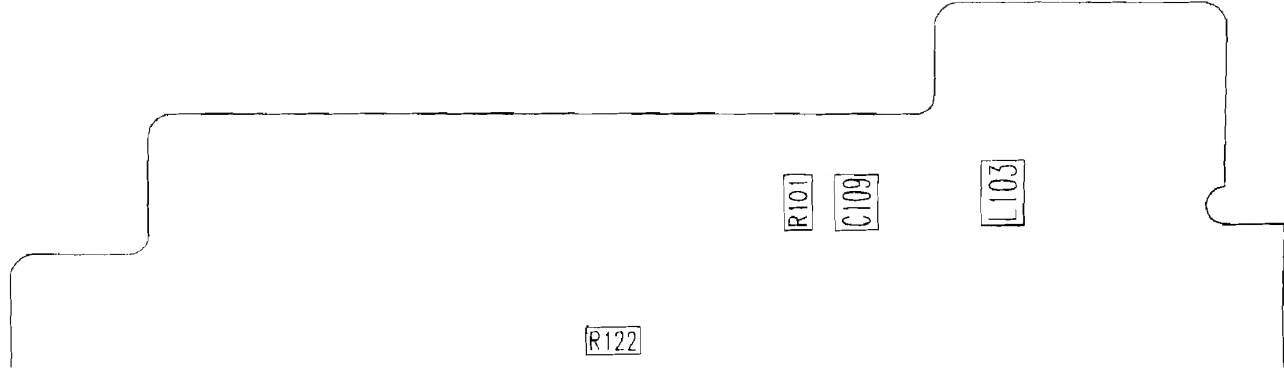


A BOTTOM

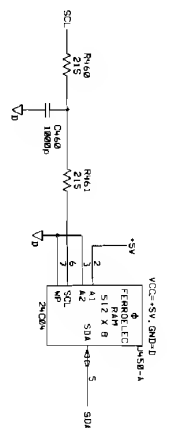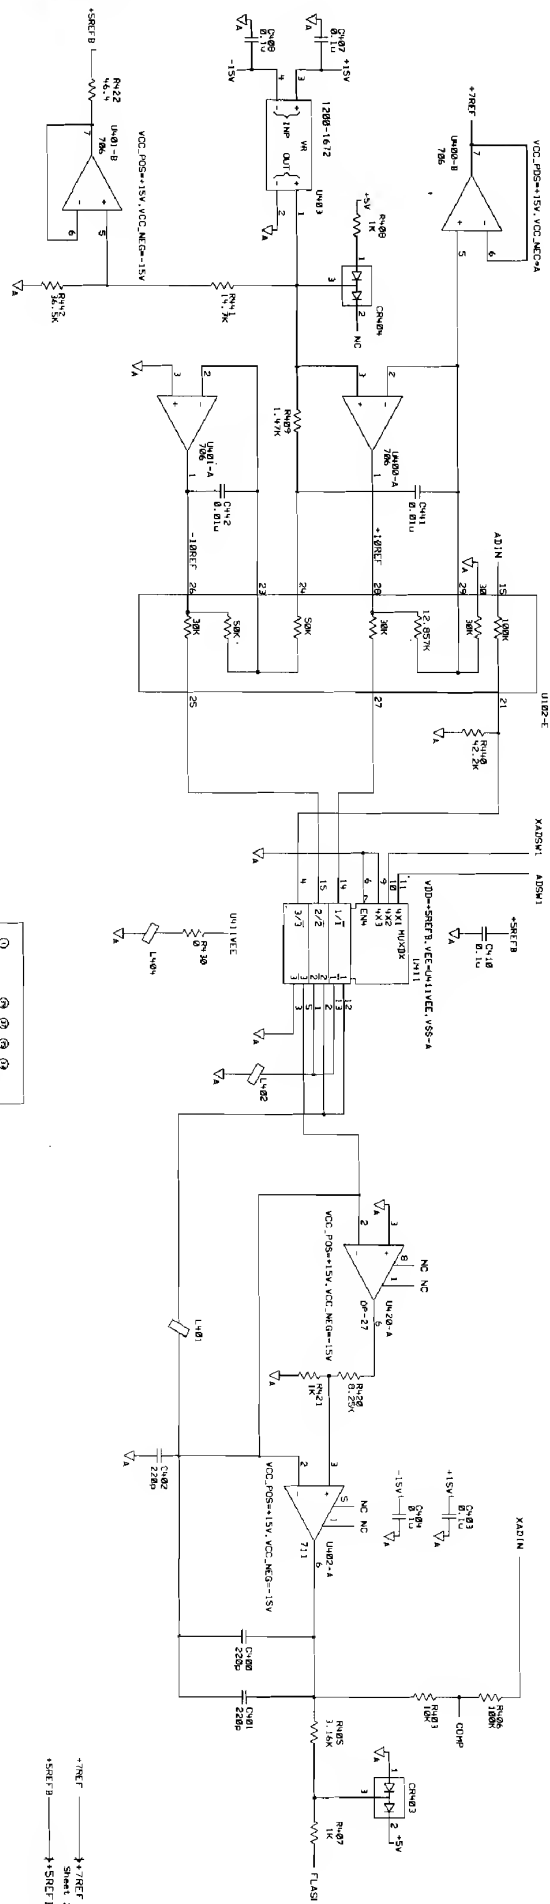



34901-66501 Rev E

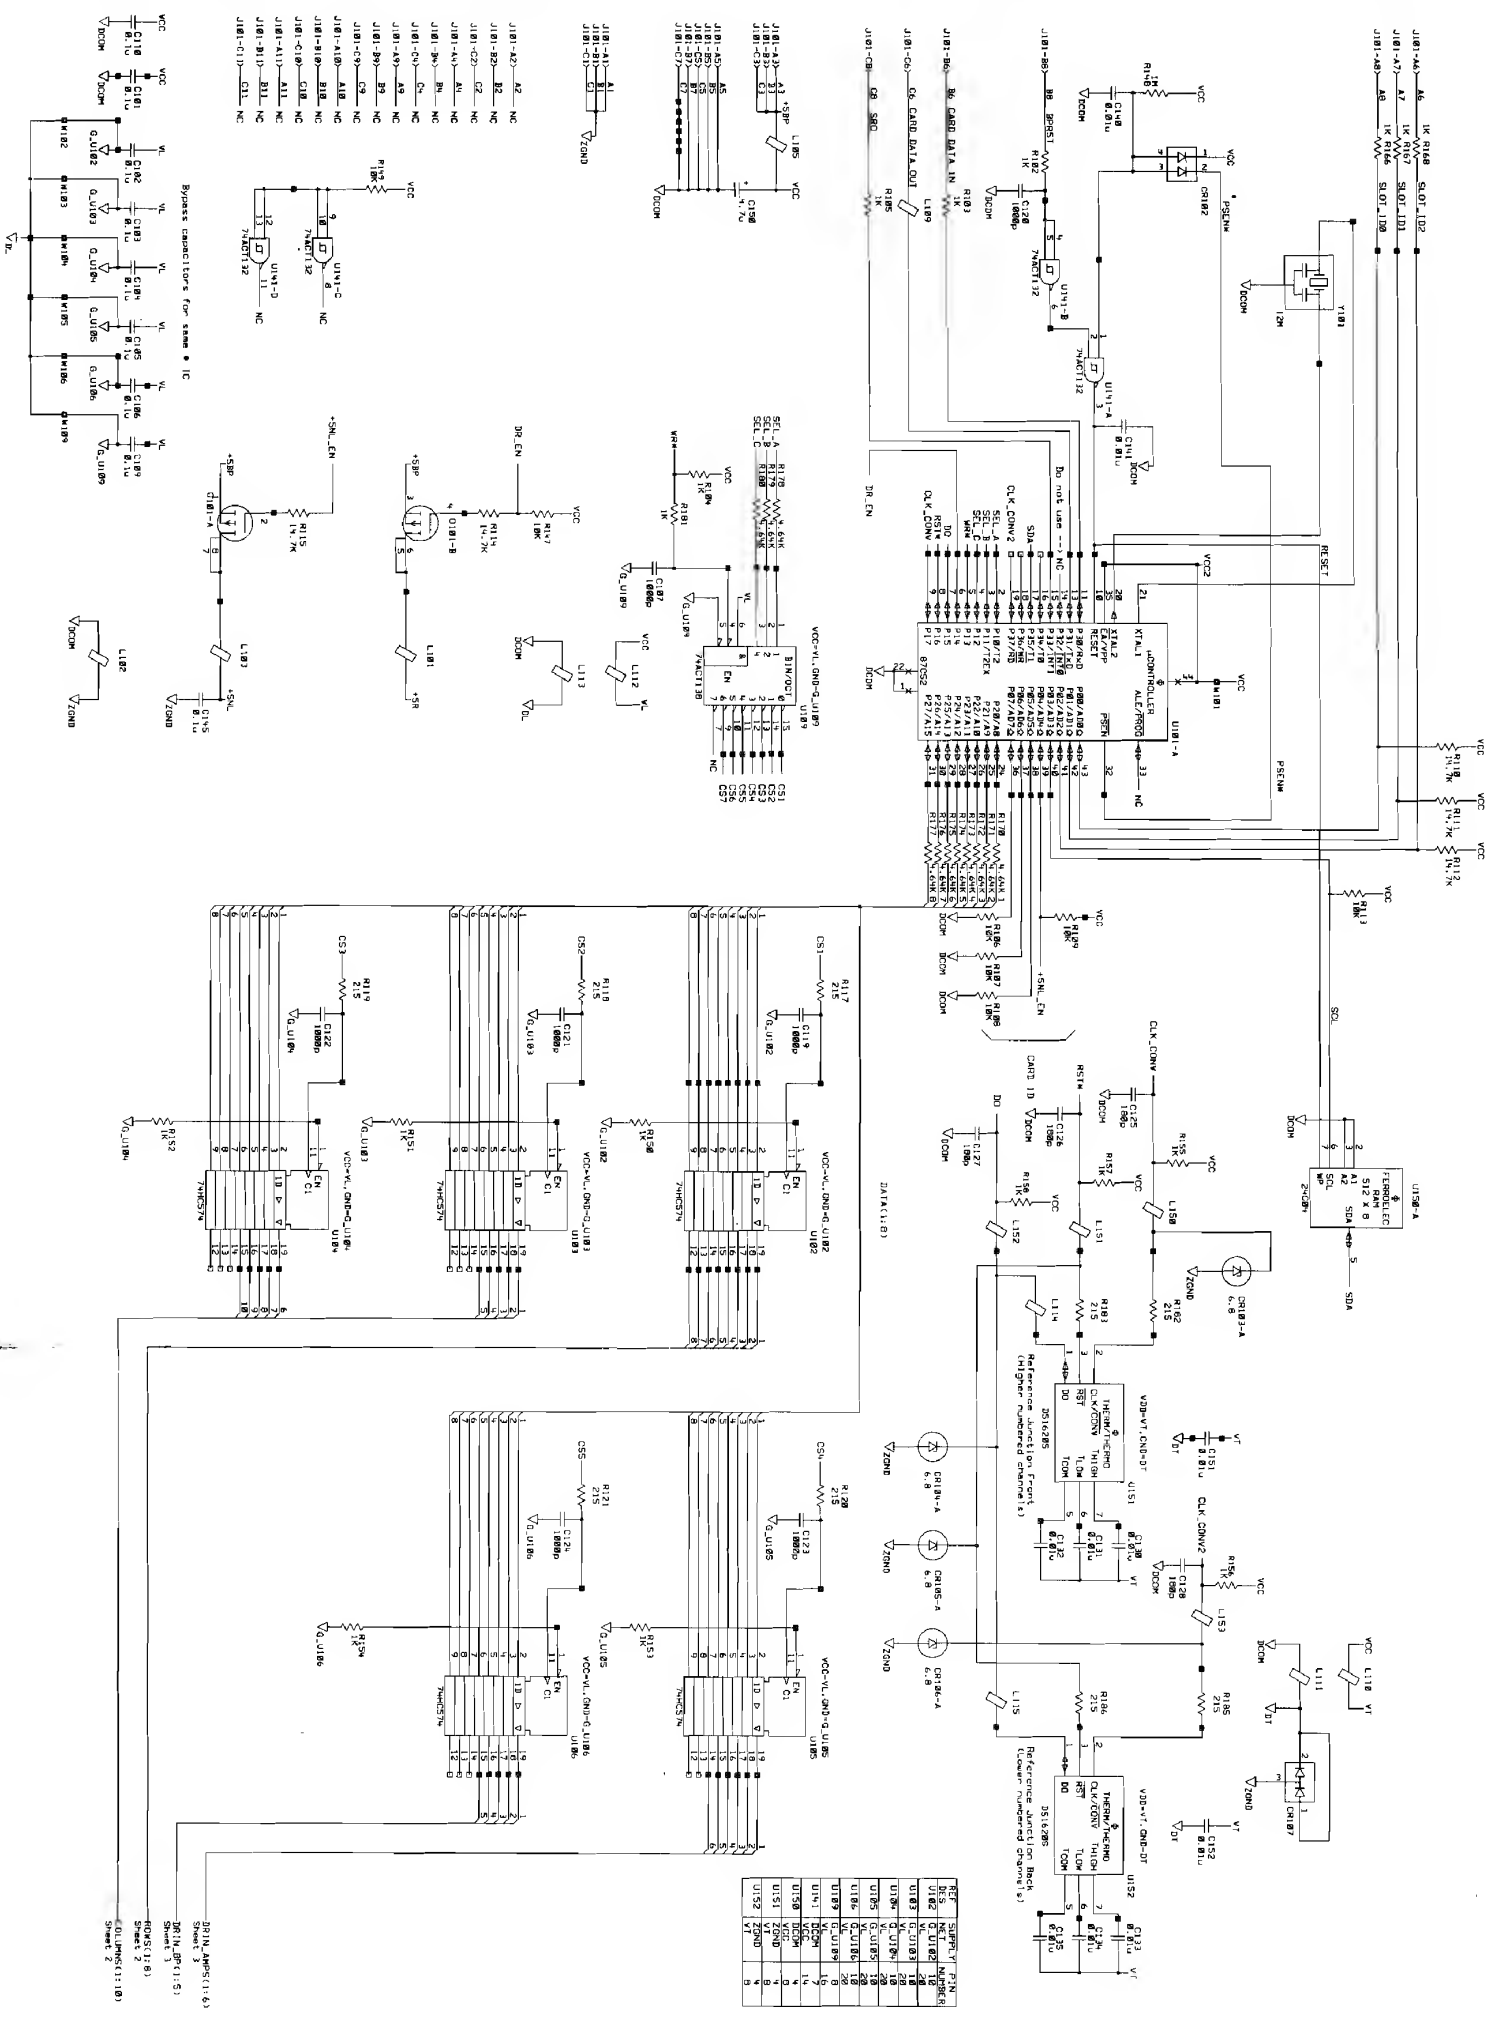


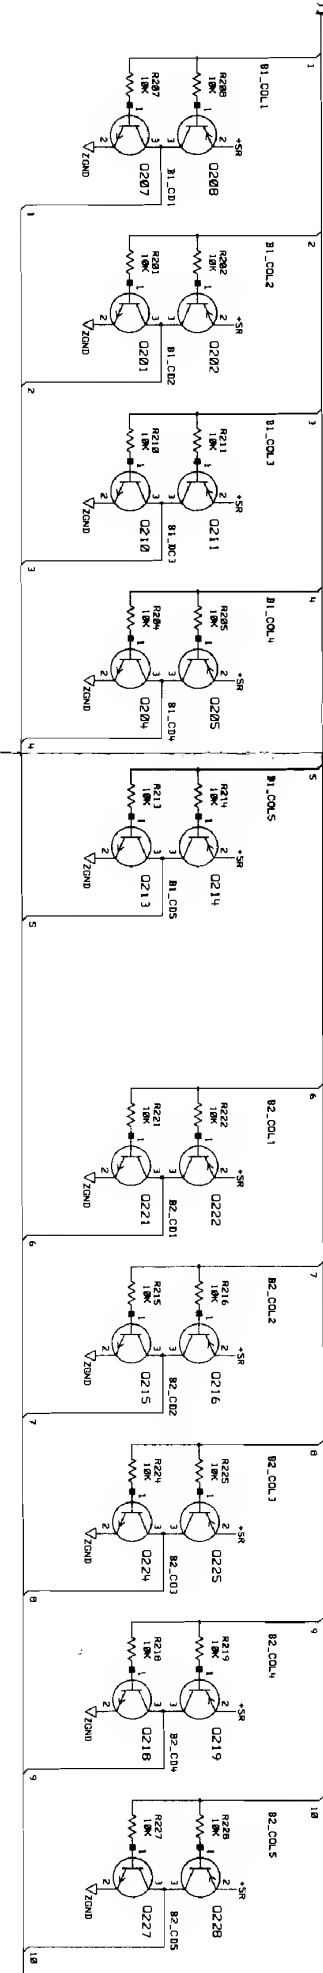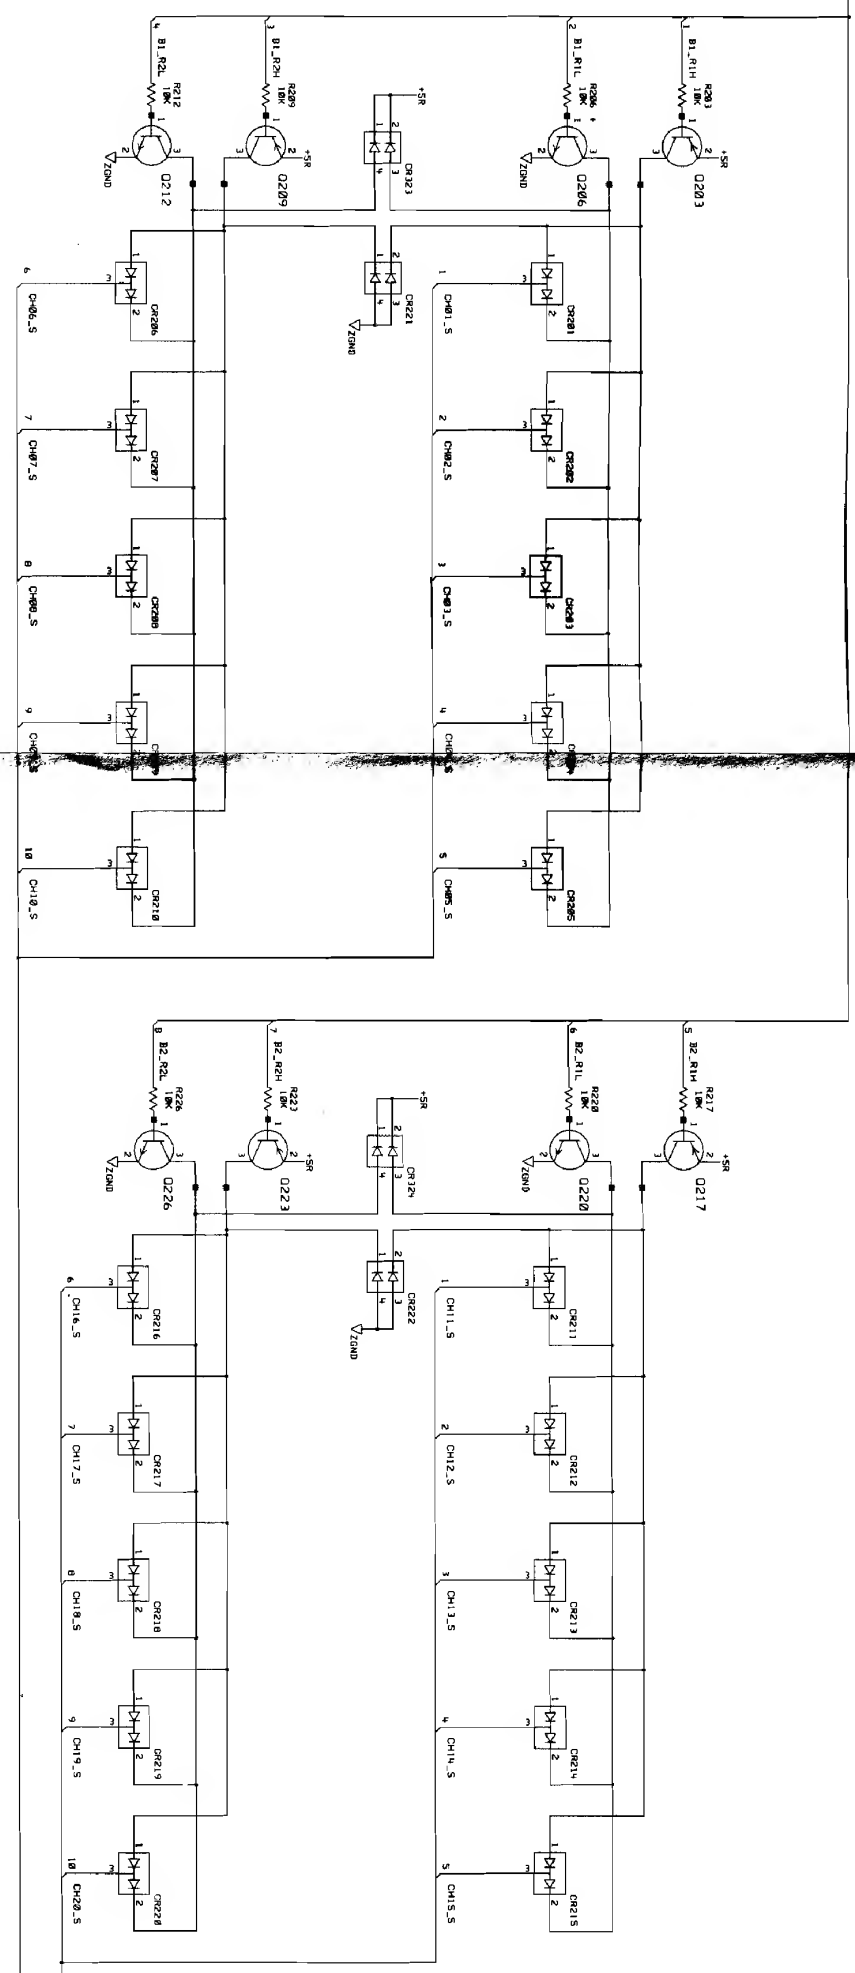


Bypass caps to be spread out among relays




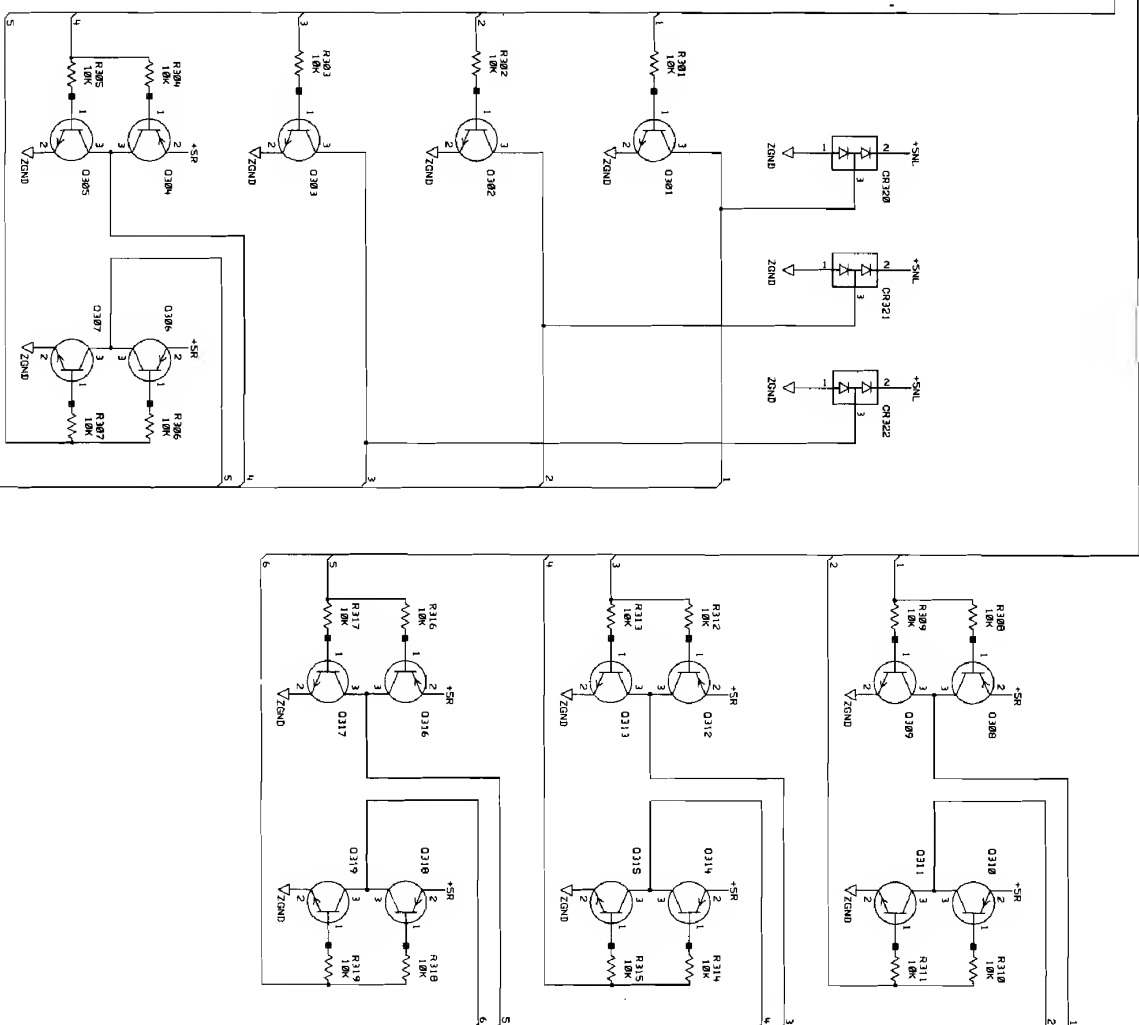

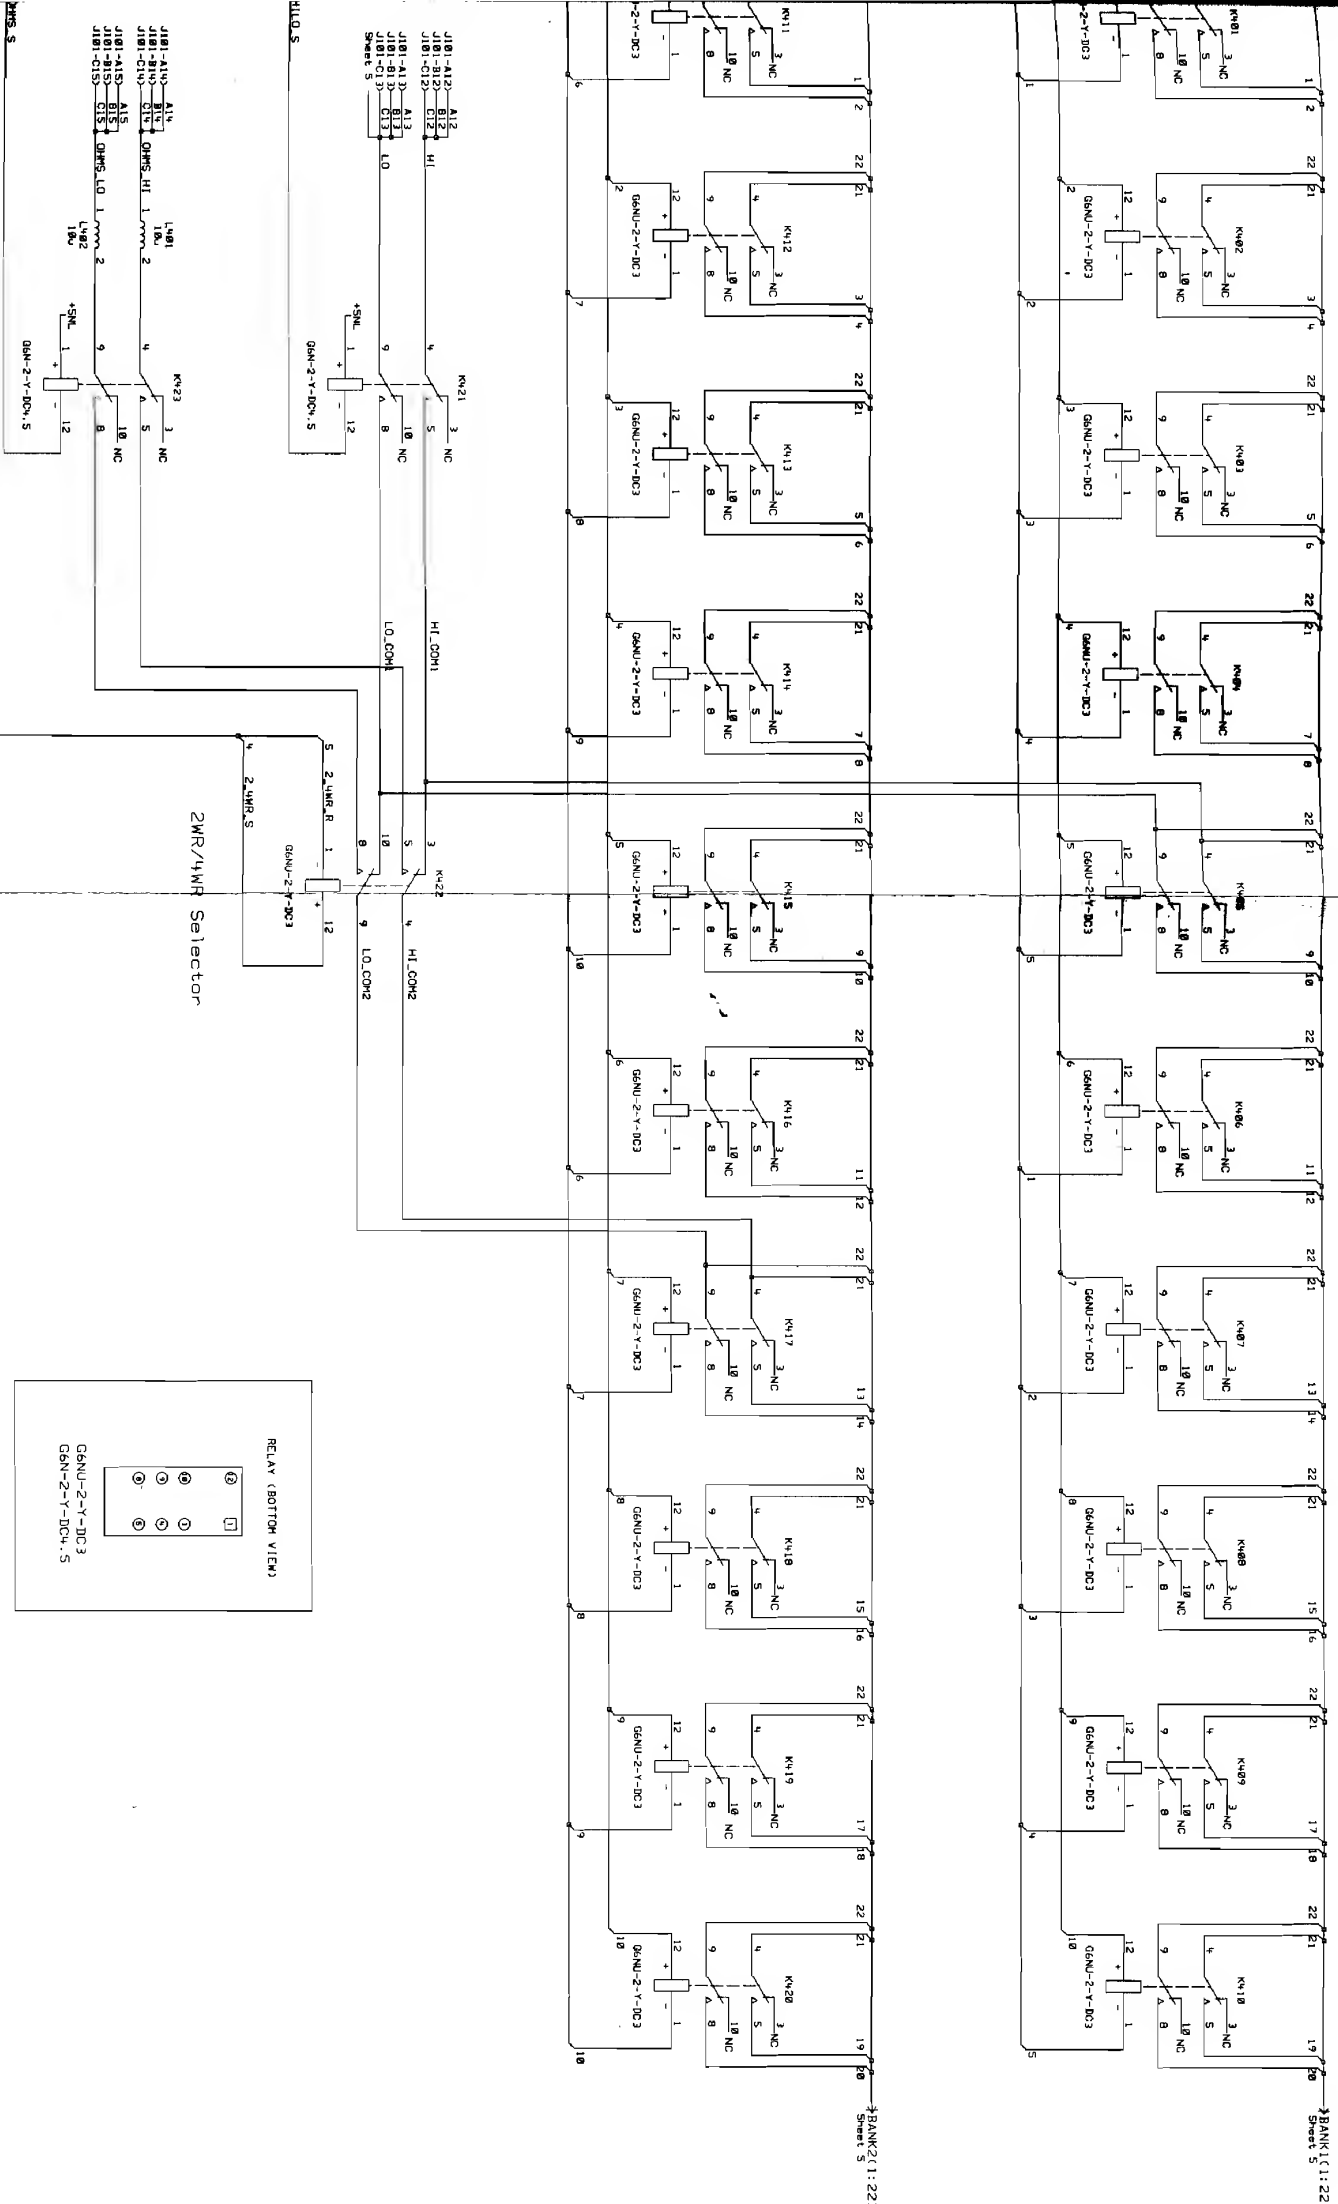

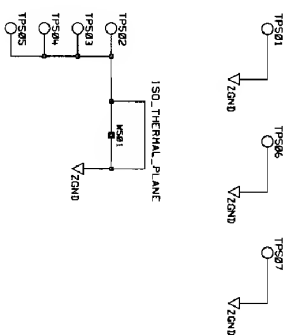

1 CH ₃ ·H ₁	102-1	9 CH ₃ ·H ₁ 9	102-9	17 CH ₃ ·H ₁ 6	101-6
2 CH ₃ ·LO 2	102-2	10 CH ₃ ·LO 10	102-10	18 CH ₃ ·LO 7	101-7
3 CH ₃ ·H ₁ 3	102-3	11 CH ₃ ·H ₁ 11	102-11	19 CH ₃ ·H ₁ 8	101-8
4 CH ₃ ·LO 4	102-4	12 CH ₃ ·LO 12	102-12	20 CH ₃ ·LO 9	101-9
5 CH ₃ ·H ₁ 5	102-5	13 CH ₃ ·H ₁ 2	101-2	21 H ₁ ·OH ₁ 4	105-4
6 CH ₃ ·LO 6	102-6	14 CH ₃ ·LO 3	101-3	22 LO·OH ₁ 3	105-3
7 CH ₃ ·H ₁ 7	102-7	15 CH ₃ ·H ₁ 4	101-4	23 CH ₃ ·LO 5	101-5
8 CH ₃ ·LO 8	102-8				



Q216 R132
CR208 R131
Q215 R130
Q214 R129
CR207 R128
R162
C162
W104
U104
C104 R114 R127
R126

C105
C106
C107
C108
C109
C110
C111
C112
R124
R123
Q207
C213

R151
C161
W103
U103
C103 R151
R122
Q206
CR203
R121
Q205

R120
Q204
CR202
R119
Q203
C212

R160
C160
W102
U102
C102 R150
R118
Q202
CR201
R117
Q201

Q218
CR210
Q220
Q217
CR209
Q213
Q212
CR206
Q211
Q210
CR205
Q209
CR211
Q208
CR204

R134
C214
R135
R133
R129
R128
R125
R124
R123

Q207
C213
Q206
CR203
R121
Q205

R120
Q204
CR202
R119
Q203
C212

R160
C160
W102
U102
C102 R150
R118
Q202
CR201
R117
Q201

K313
K312
K311
K310
K309
K308
K307
K306
K305
K304
K303
K302
K301

C403

R404 R403

C402

R401 R402

C401

R400

TP403
R111
R110
R109
R108
U151
R107
R106
TP405

TP400

TP407
R115
R114
R113
R112
U152
R111
R110
R109
R108
TP408

TP401

J101

L301

L302

L104

R149

U141

R102

C120

C141

R168

R156

R157

R105

R109

R103

C150

L102

R115

R140

C140

R148

CR102

Y101

R124

R136

R126

R132

R121

R137

R141

R139

R122

R133

R127

R138

R125

R135

R123

R131

U101

U150

W103

R107

R116

R118

R105

R110

R112

R114

R117

R119

L101

Q101

L112

L113

L300

K316

K328

K315

K327

K314


K326


CR107

CR105




CR103

CR104

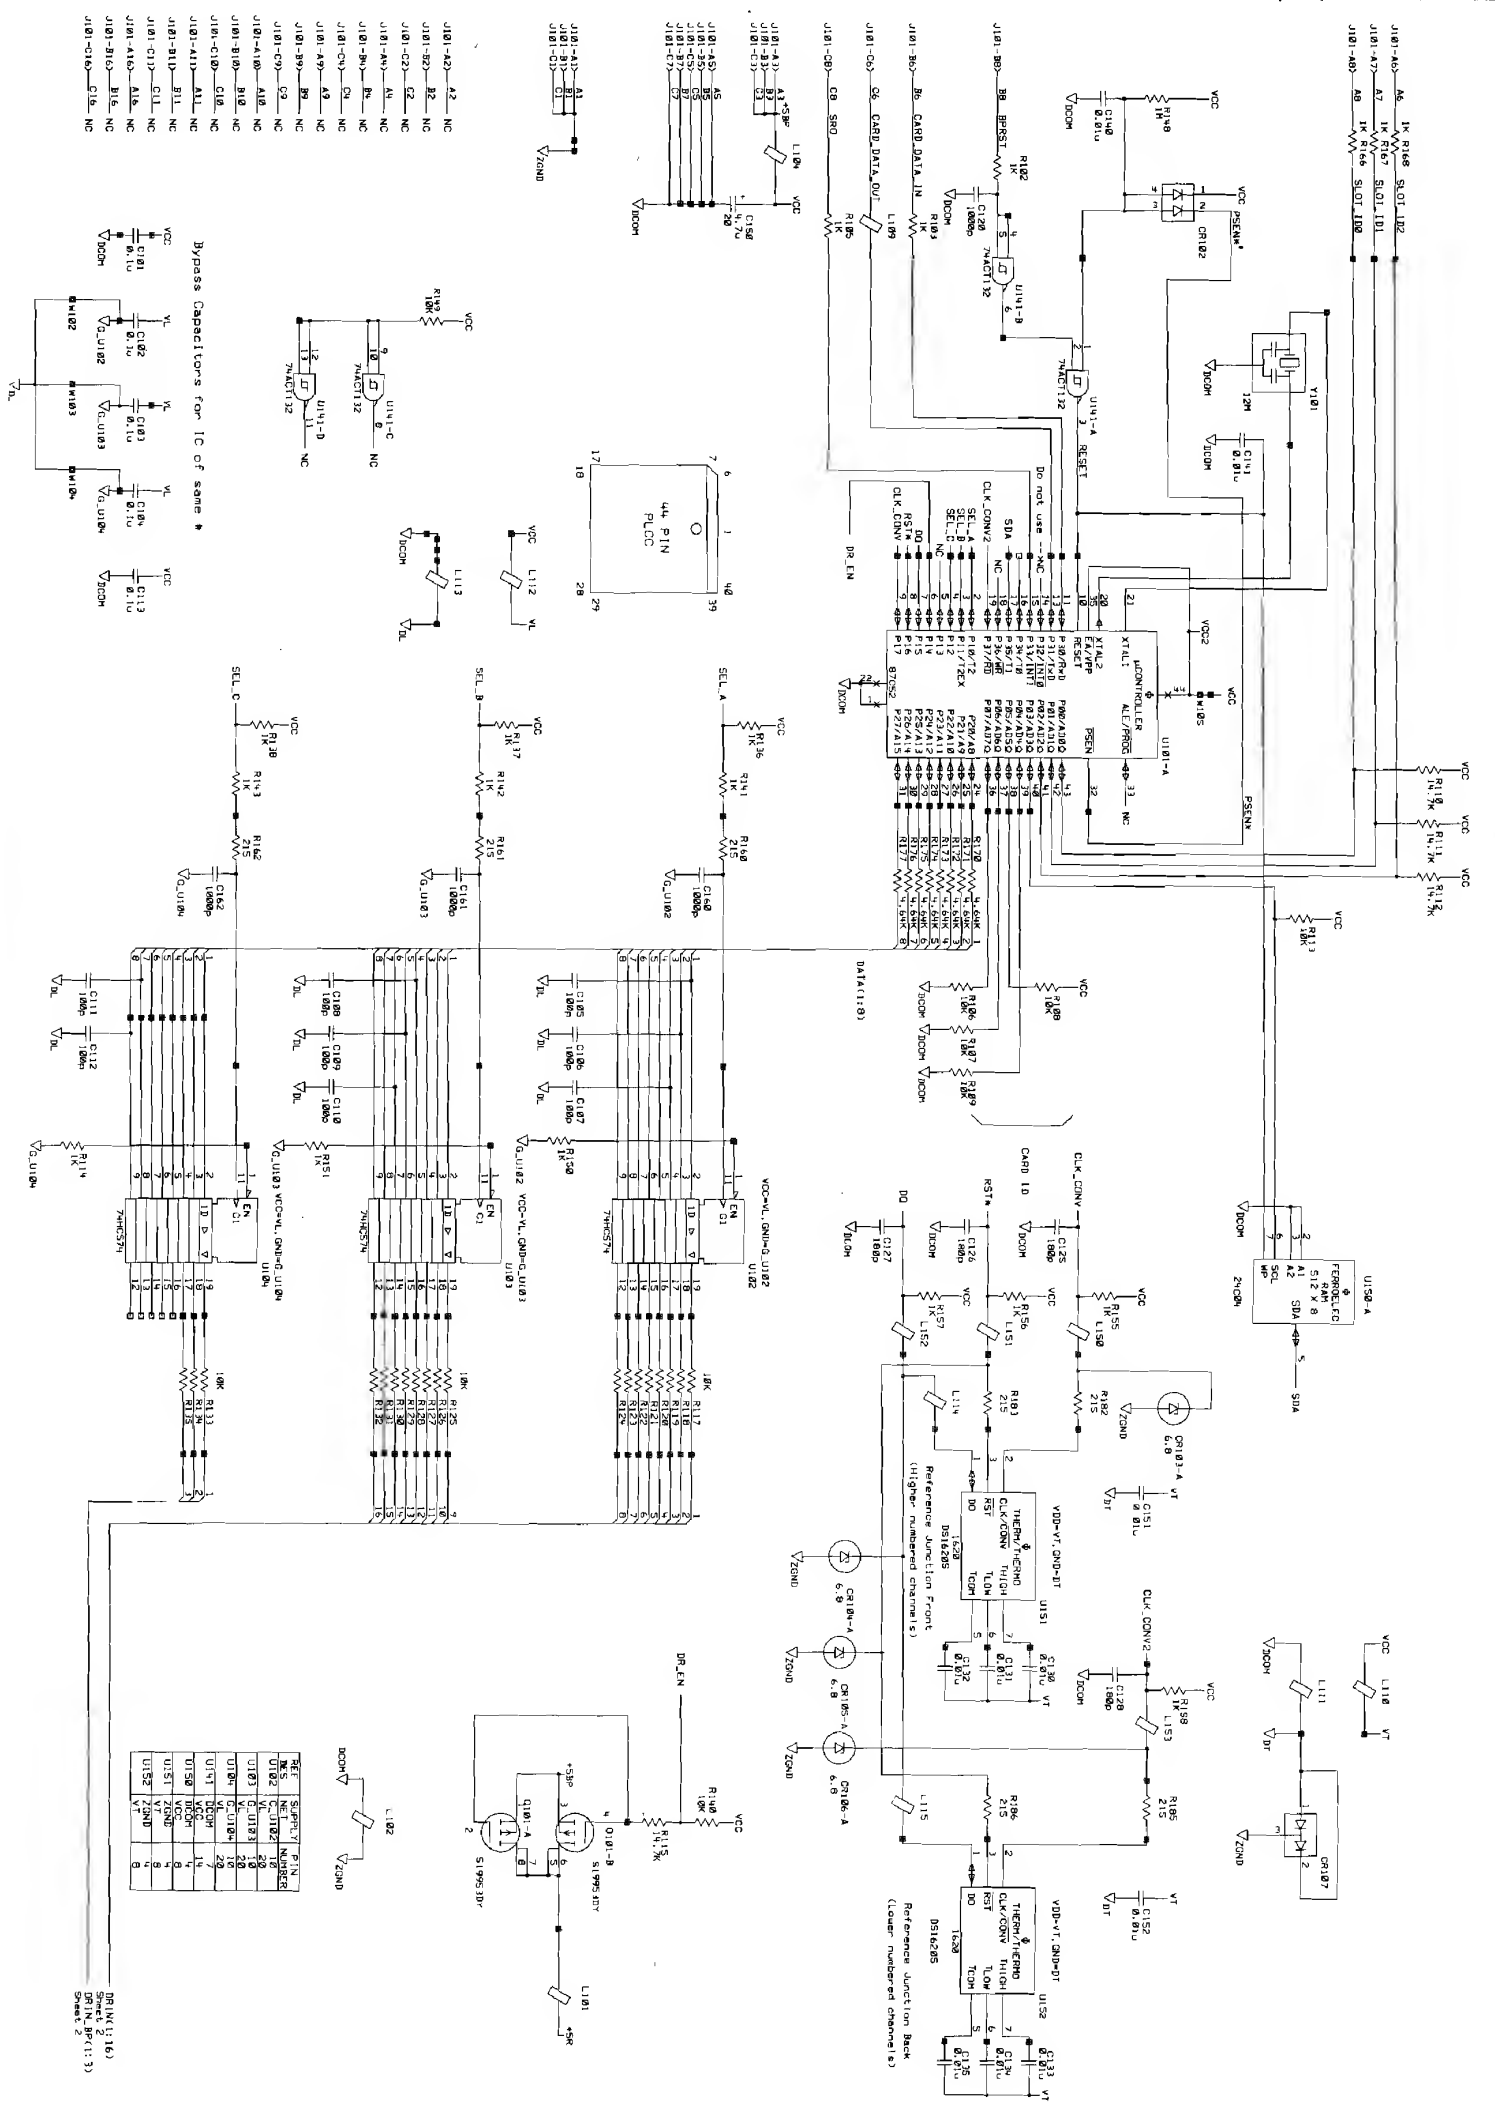

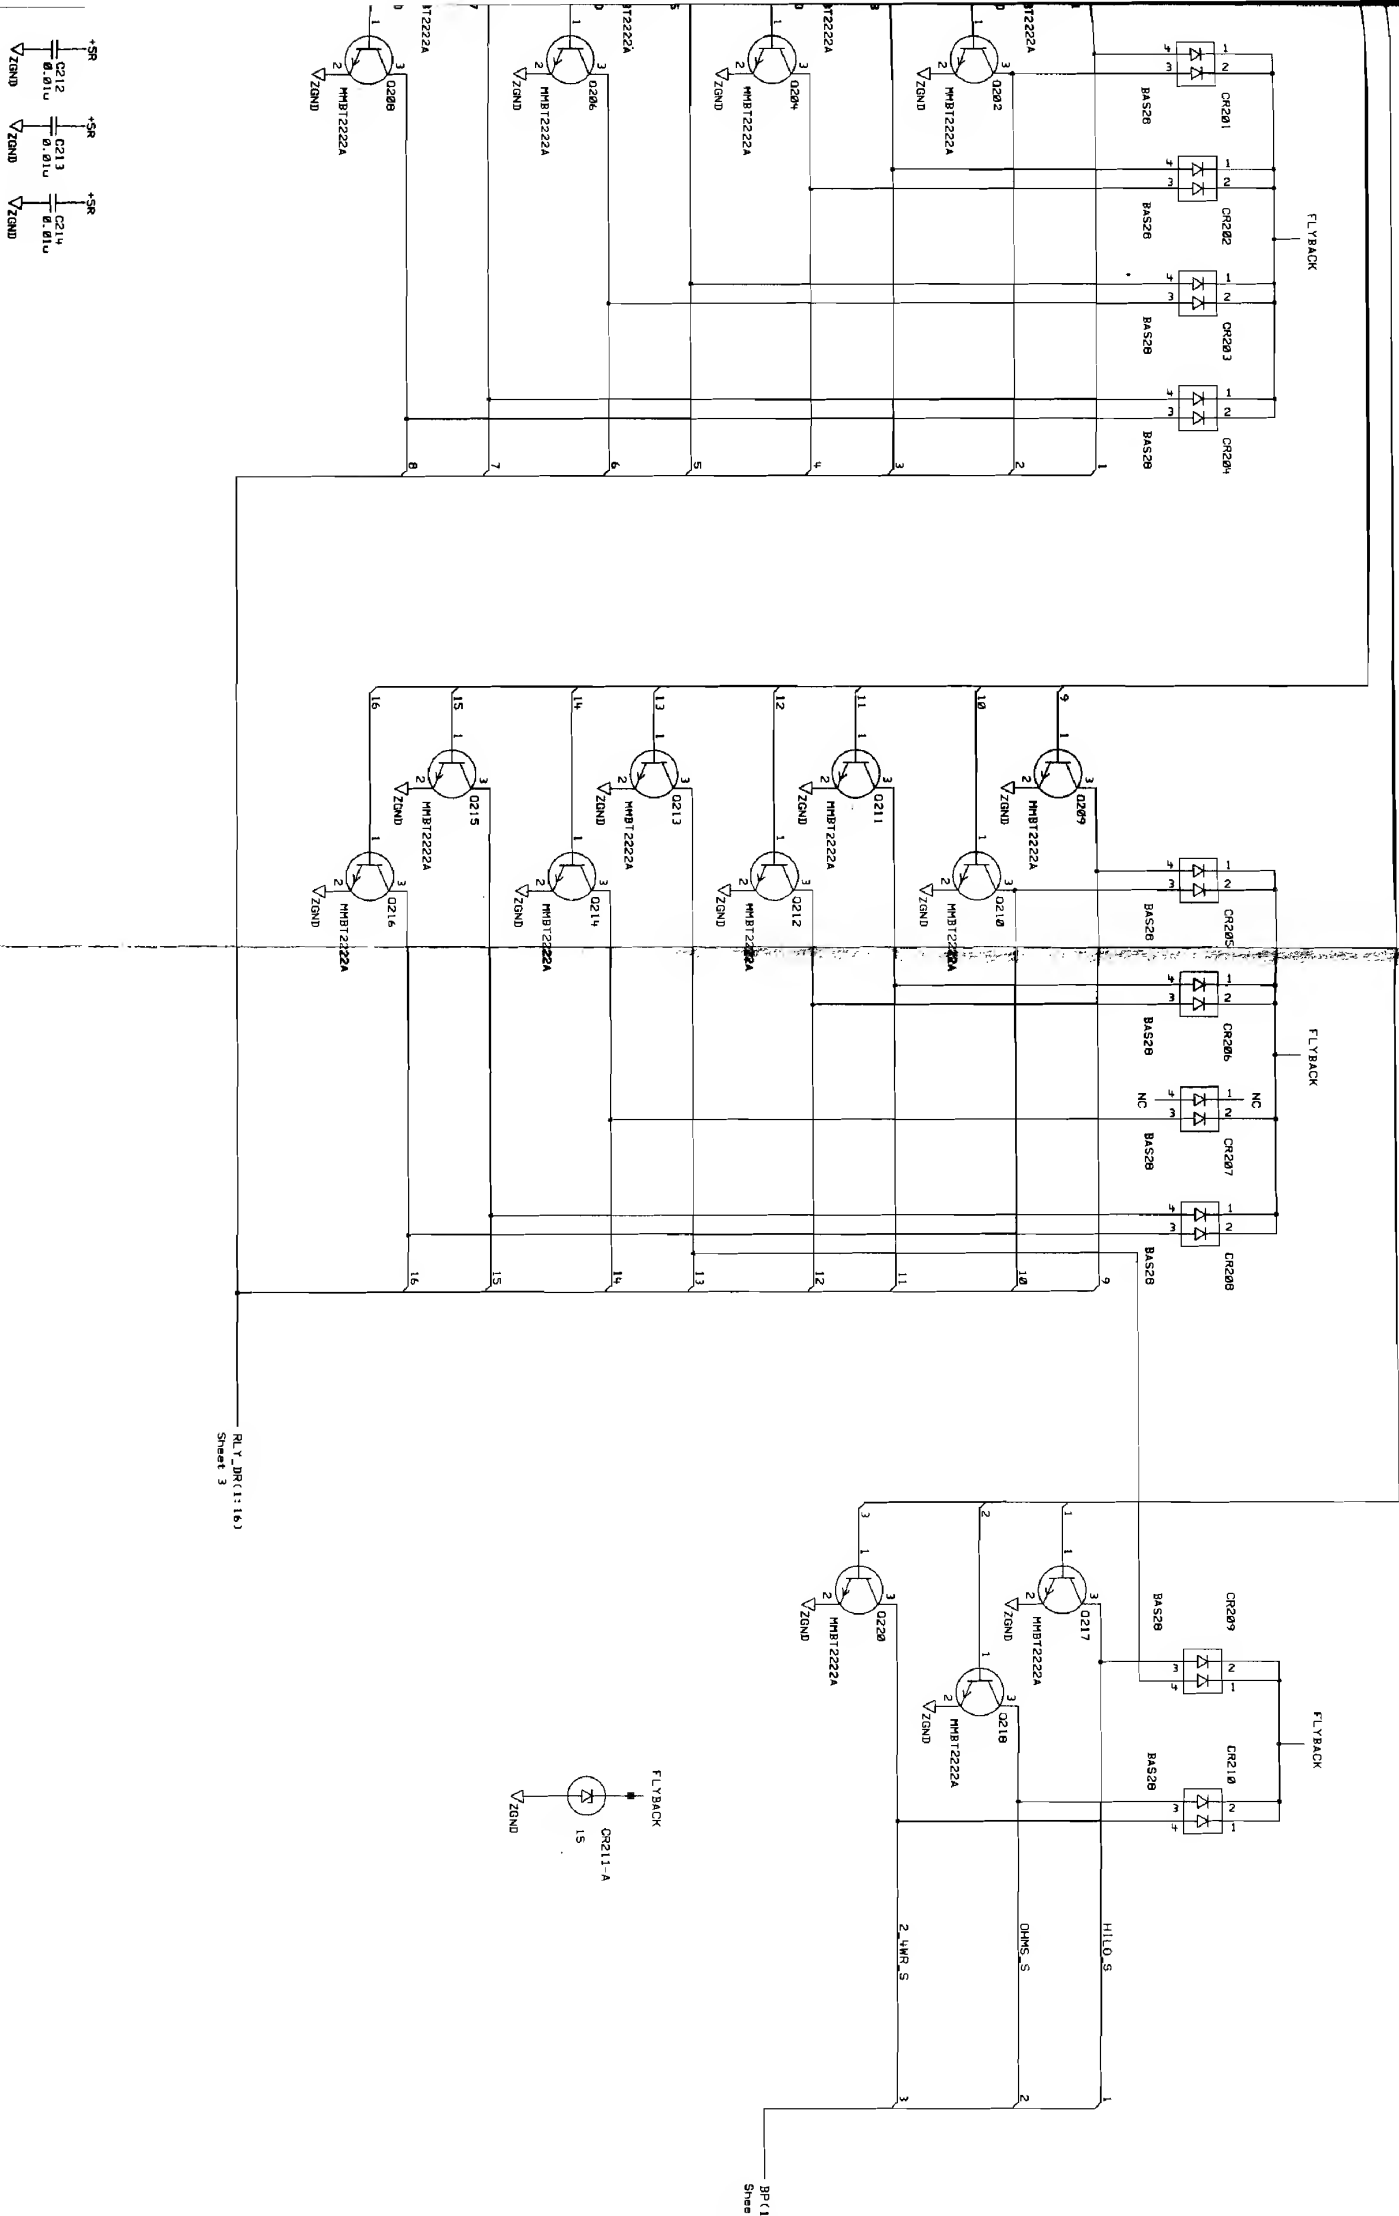

USER CONNECTORS

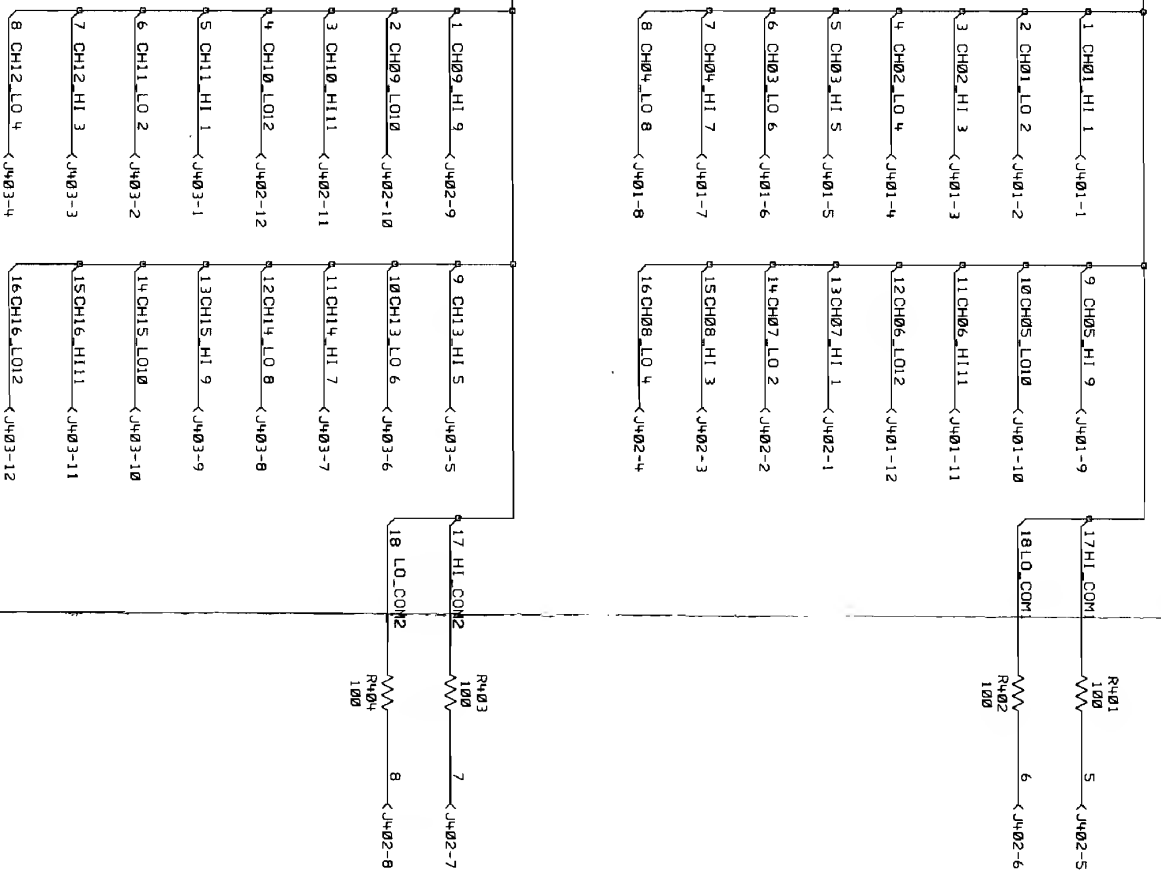

150-THERMAL PLACES

BANK 1:18
Sheet 3
BANK 2:1:18
Sheet 3

J101

L102

C150

L101

Q101

L110

L111

L103

R107
R102
R105
R103
R109
R106
R108
R104

C141

CR103

Y101

R127
R124

R170
R171
R172
R173
R174
R175

U101

R176
R177

R106
R107
R108
R109
R178
R179

R149

U141

CR102

R148
R140

U150

R110
R111
R112
R113
R172
R173
R174
R175

Q228
CR220

K320

Q227

CR219

K319

Q226

Q225
CR218

K318

Q224

CR217

K317

Q223

CR225

K316

Q222

CR216

K315

Q221

CR222

K314

Q220

CR215

K313

Q219

CR214

K312

Q218

CR213

K311

Q217

CR212

K310

Q216

CR211

K309

Q215

CR210

K308

Q214

CR209

K307


Q213

CR208

K306

U304

U305



R118
R119

W104

U104

R114

C125

C123

C121


C126

C127




C124

34903-66501 Rev B

HP 34903A 20-Channel Actuator Component Locator

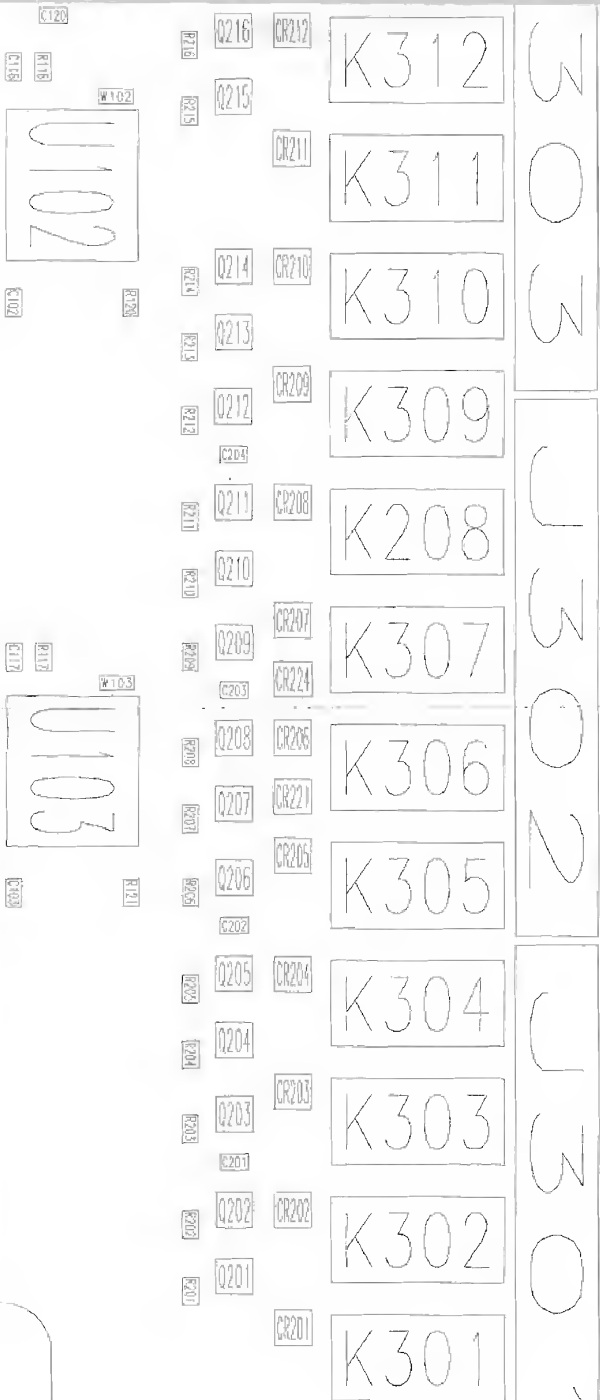



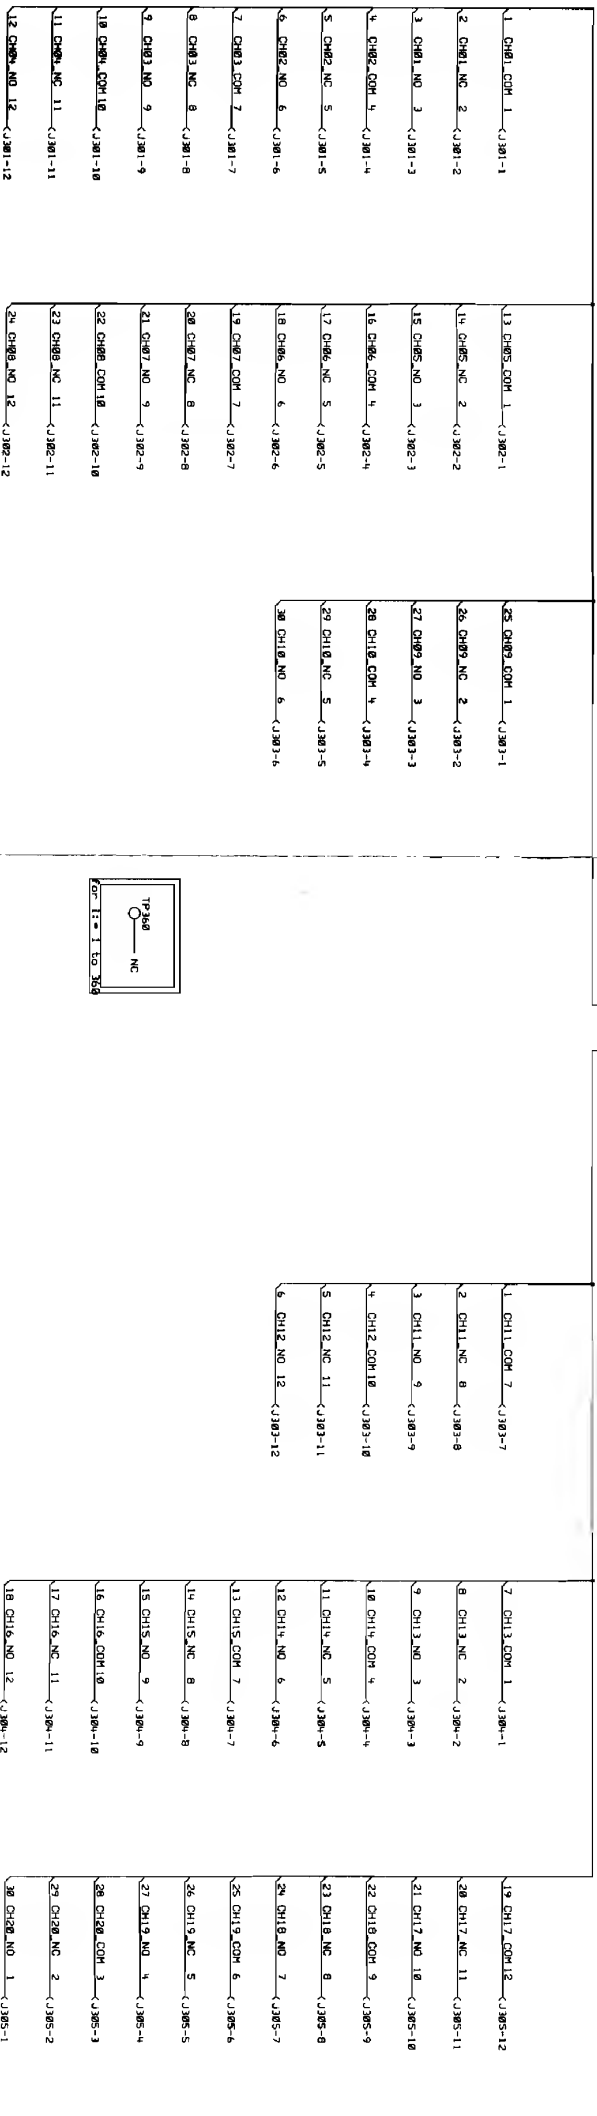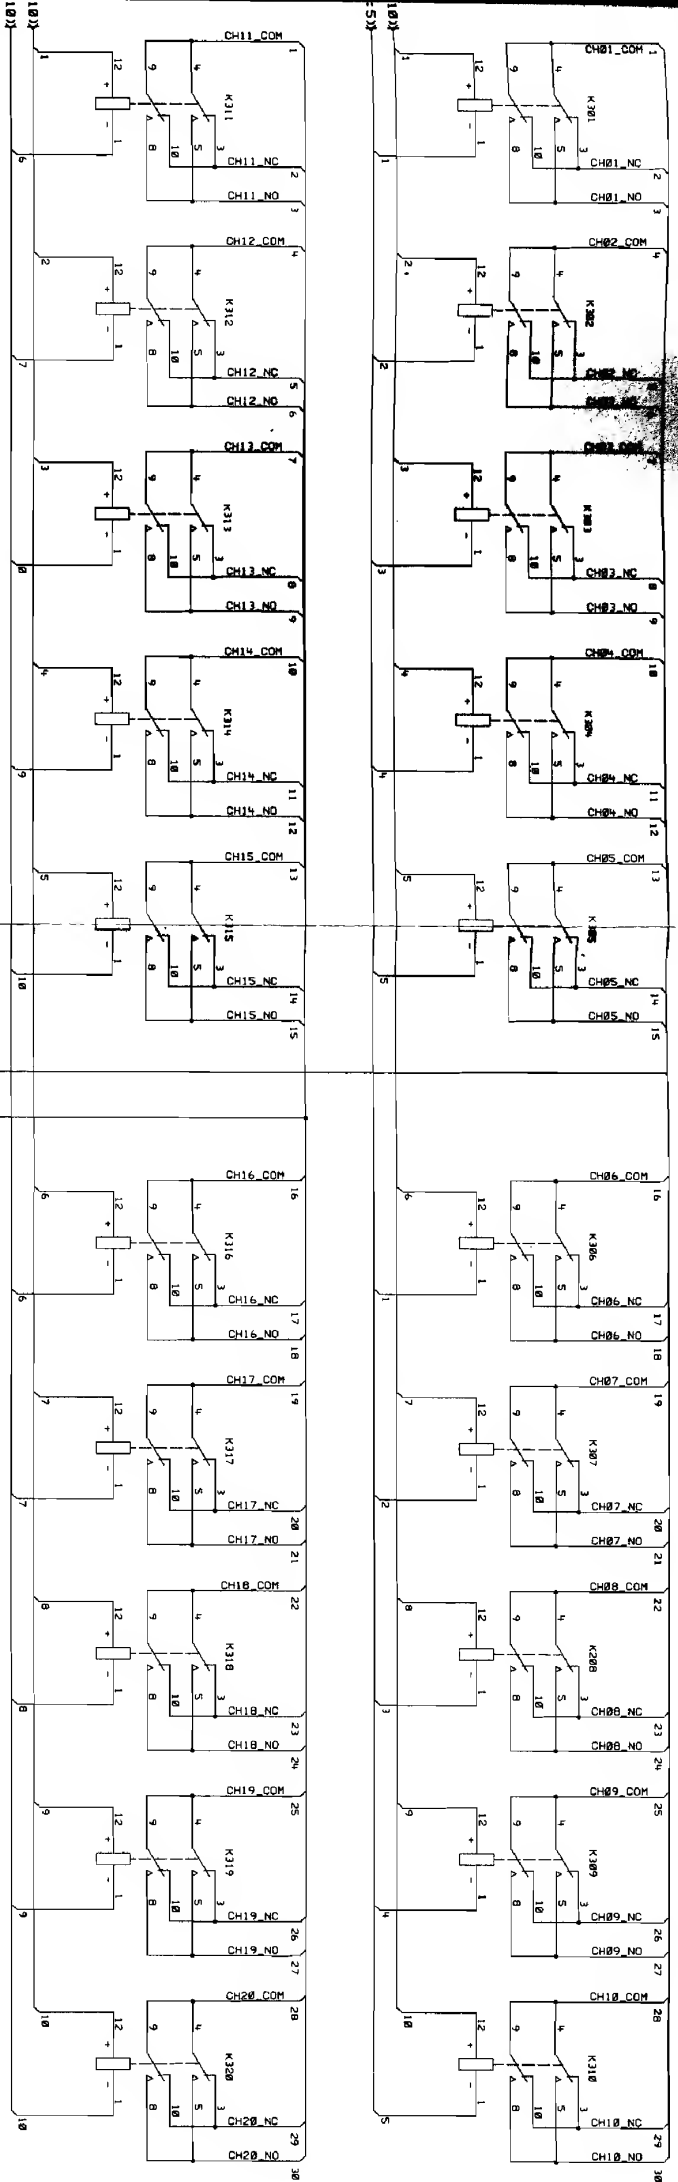

U101

L106 L107 L108

L105

R151 R152 R153 R154 R155 R156 R157 R158

U141

U111

CR109

R148 R149

C158

R213 R156 R157

U101

Y101

CR409

R147

Q101

C157

L101

C156 C159 R158 R159 R160 R161 R162 R163 R164

R287

C164

C165 C166 R165

U103

R164

U102

C154

R173 R171 R172 R174
Q133 Q131 Q143 Q141

R171 R173 R172 R174
Q111 Q113 Q121 Q123

Q204 Q201 Q211 Q213
CR301 CR401

CR111 Q223 Q221 Q233
CR302 CR402

Q231 Q233 Q234 Q235
CR303 CR403

K401 K301 K201 K101

K402 K302 K202 K102

K403 K303 K203 K103

CR101 CR201 CR102 CR202

CR110

J102

J103

TP305

TP304

TP383

TP382

CR103 CR203

CR104 CR204

CR105 CR205

CR106 CR206

Q205

J104

J105

CR107 CR207

CR108 CR208

Q207

TP381

K104

K105

K106

K107

K108

K204

K205

K206

K207

K208

K304

K305

K306

K307

K308

K404

K405

K406

K407

K408

J106

J107

Q243

Q241

CR404

Q253

Q251

CR405

Q263

Q261

CR406

Q273

Q271

CR407

Q283

Q281

CR408

TP306

R243

R241

CR304

R253

R251

CR305

R263

R261

CR306

R273

R271


CR307

R283


R281

CR308

34904-66501 Rev A

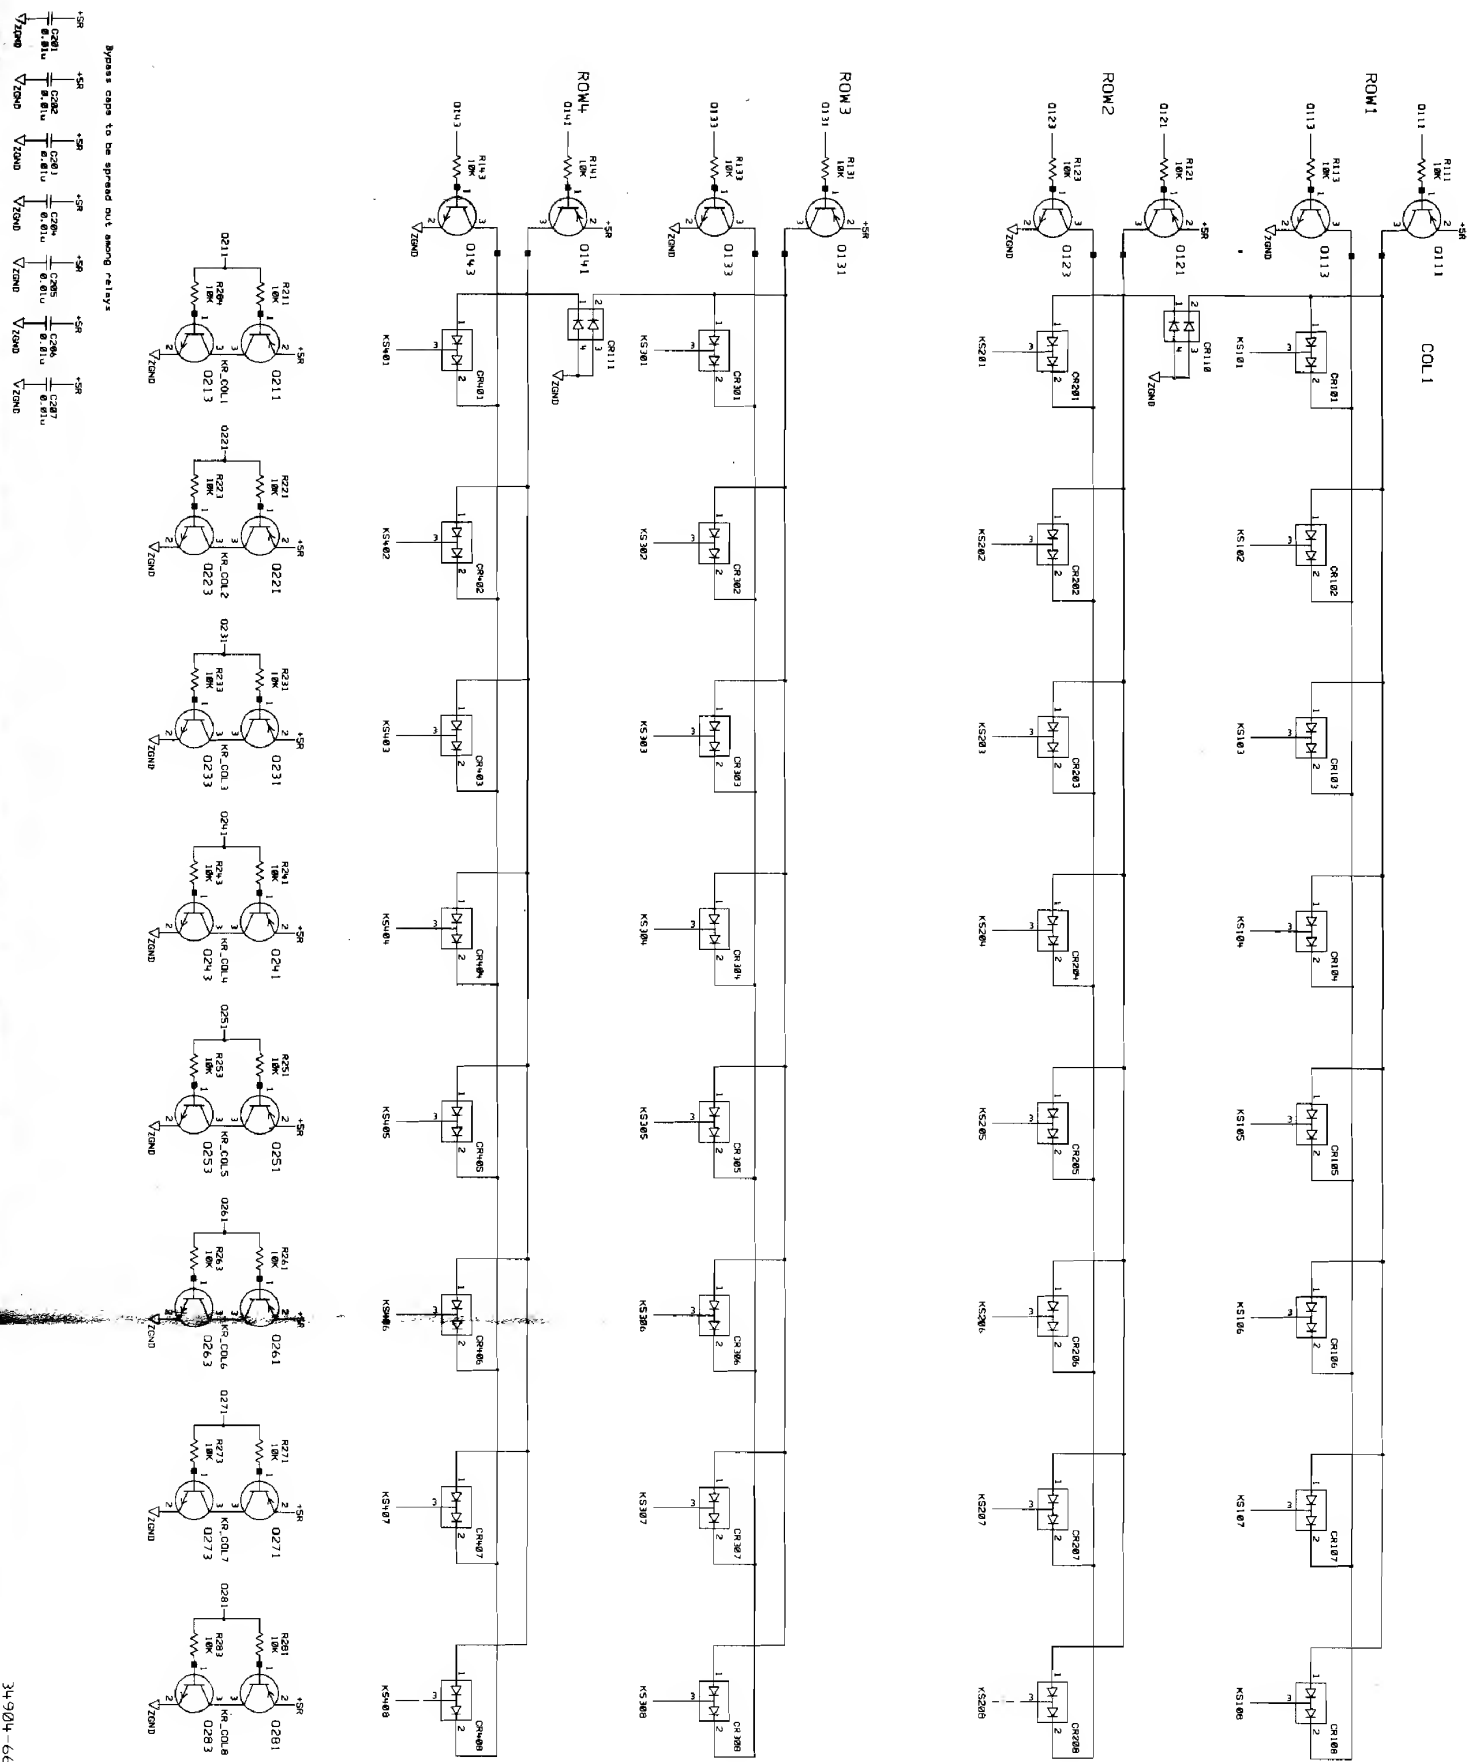


Bypass caps to be spread out along relays




Earth referenced holes for shielding



COL 1 COL 2 COL 3 COL 4 COL 5 COL 6 COL 7 COL 8

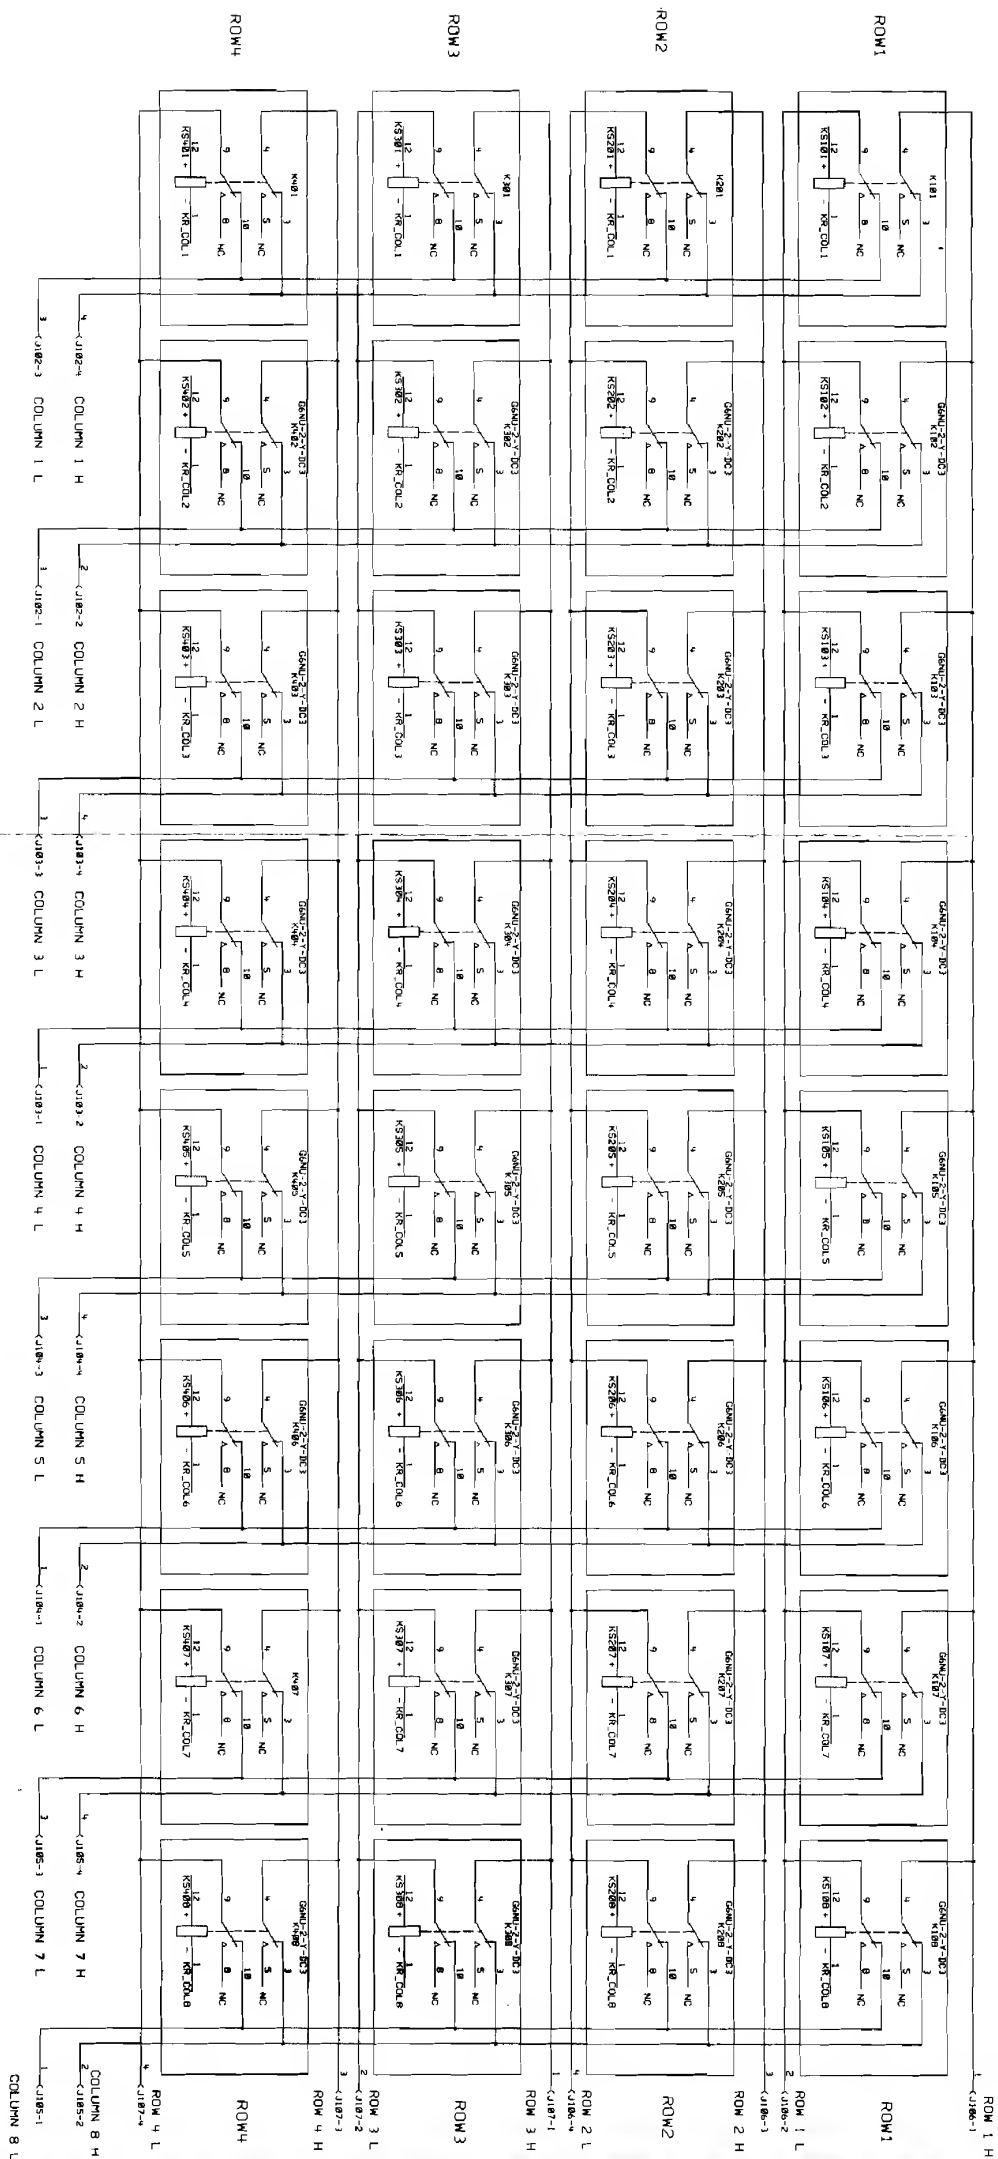

RELAY SCHEMATIC (BOTTOM VIEW)



G6NU-2-V-DC3

U101

U141

R119

U111

CR102

R148 C140

R159

C158

R158

R157

C101 R156 R155 R154 R153 R152 R151 R150 R149 R148 R147 R146 R145 R144 R143 R142 R141 R140 R139 R138 R137 R136 R135 R134 R133 R132 R131 R130 R129 R128 R127 R126 R125 R124 R123 R122 R121 R120 R119 R118 R117 R116 R115 R114 R113 R112 R111 R110 R109 R108 R107 R106 R105 R104 R103 R102 R101 R100 R099 R098 R097 R096 R095 R094 R093 R092 R091 R090 R089 R088 R087 R086 R085 R084 R083 R082 R081 R080 R079 R078 R077 R076 R075 R074 R073 R072 R071 R070 R069 R068 R067 R066 R065 R064 R063 R062 R061 R060 R059 R058 R057 R056 R055 R054 R053 R052 R051 R050 R049 R048 R047 R046 R045 R044 R043 R042 R041 R040 R039 R038 R037 R036 R035 R034 R033 R032 R031 R030 R029 R028 R027 R026 R025 R024 R023 R022 R021 R020 R019 R018 R017 R016 R015 R014 R013 R012 R011 R010 R009 R008 R007 R006 R005 R004 R003 R002 R001

U101

Y101

CR170

Q170

L171

L170

C111

U102

U103

R27

C164

R164

C162

C163

C165

Q204 Q203 Q202 Q201

Q204 Q203 Q202 Q201

K202

K202

K202

P6

P7

P8

P9

P12

P11

P10
P1
P2
P3
P4
P5

Q238
Q235

Q240
Q241
Q242
Q239

Q245
Q246
Q243


Q208 Q207 Q206 Q205
R208 R207 R206 R205
Q212 Q211 Q210 Q209
R212 R211 R210 R209
R202




Q104 Q103 Q102 Q101
R104 R103 R102 R101

Q248
Q249
Q250
Q247


Q108 Q107 Q106 Q105
R108 R107 R106 R105
Q112 Q111 Q110 Q109
R112 R111 R110 R109

34905-66501 Rev A
34906-66501 Rev A

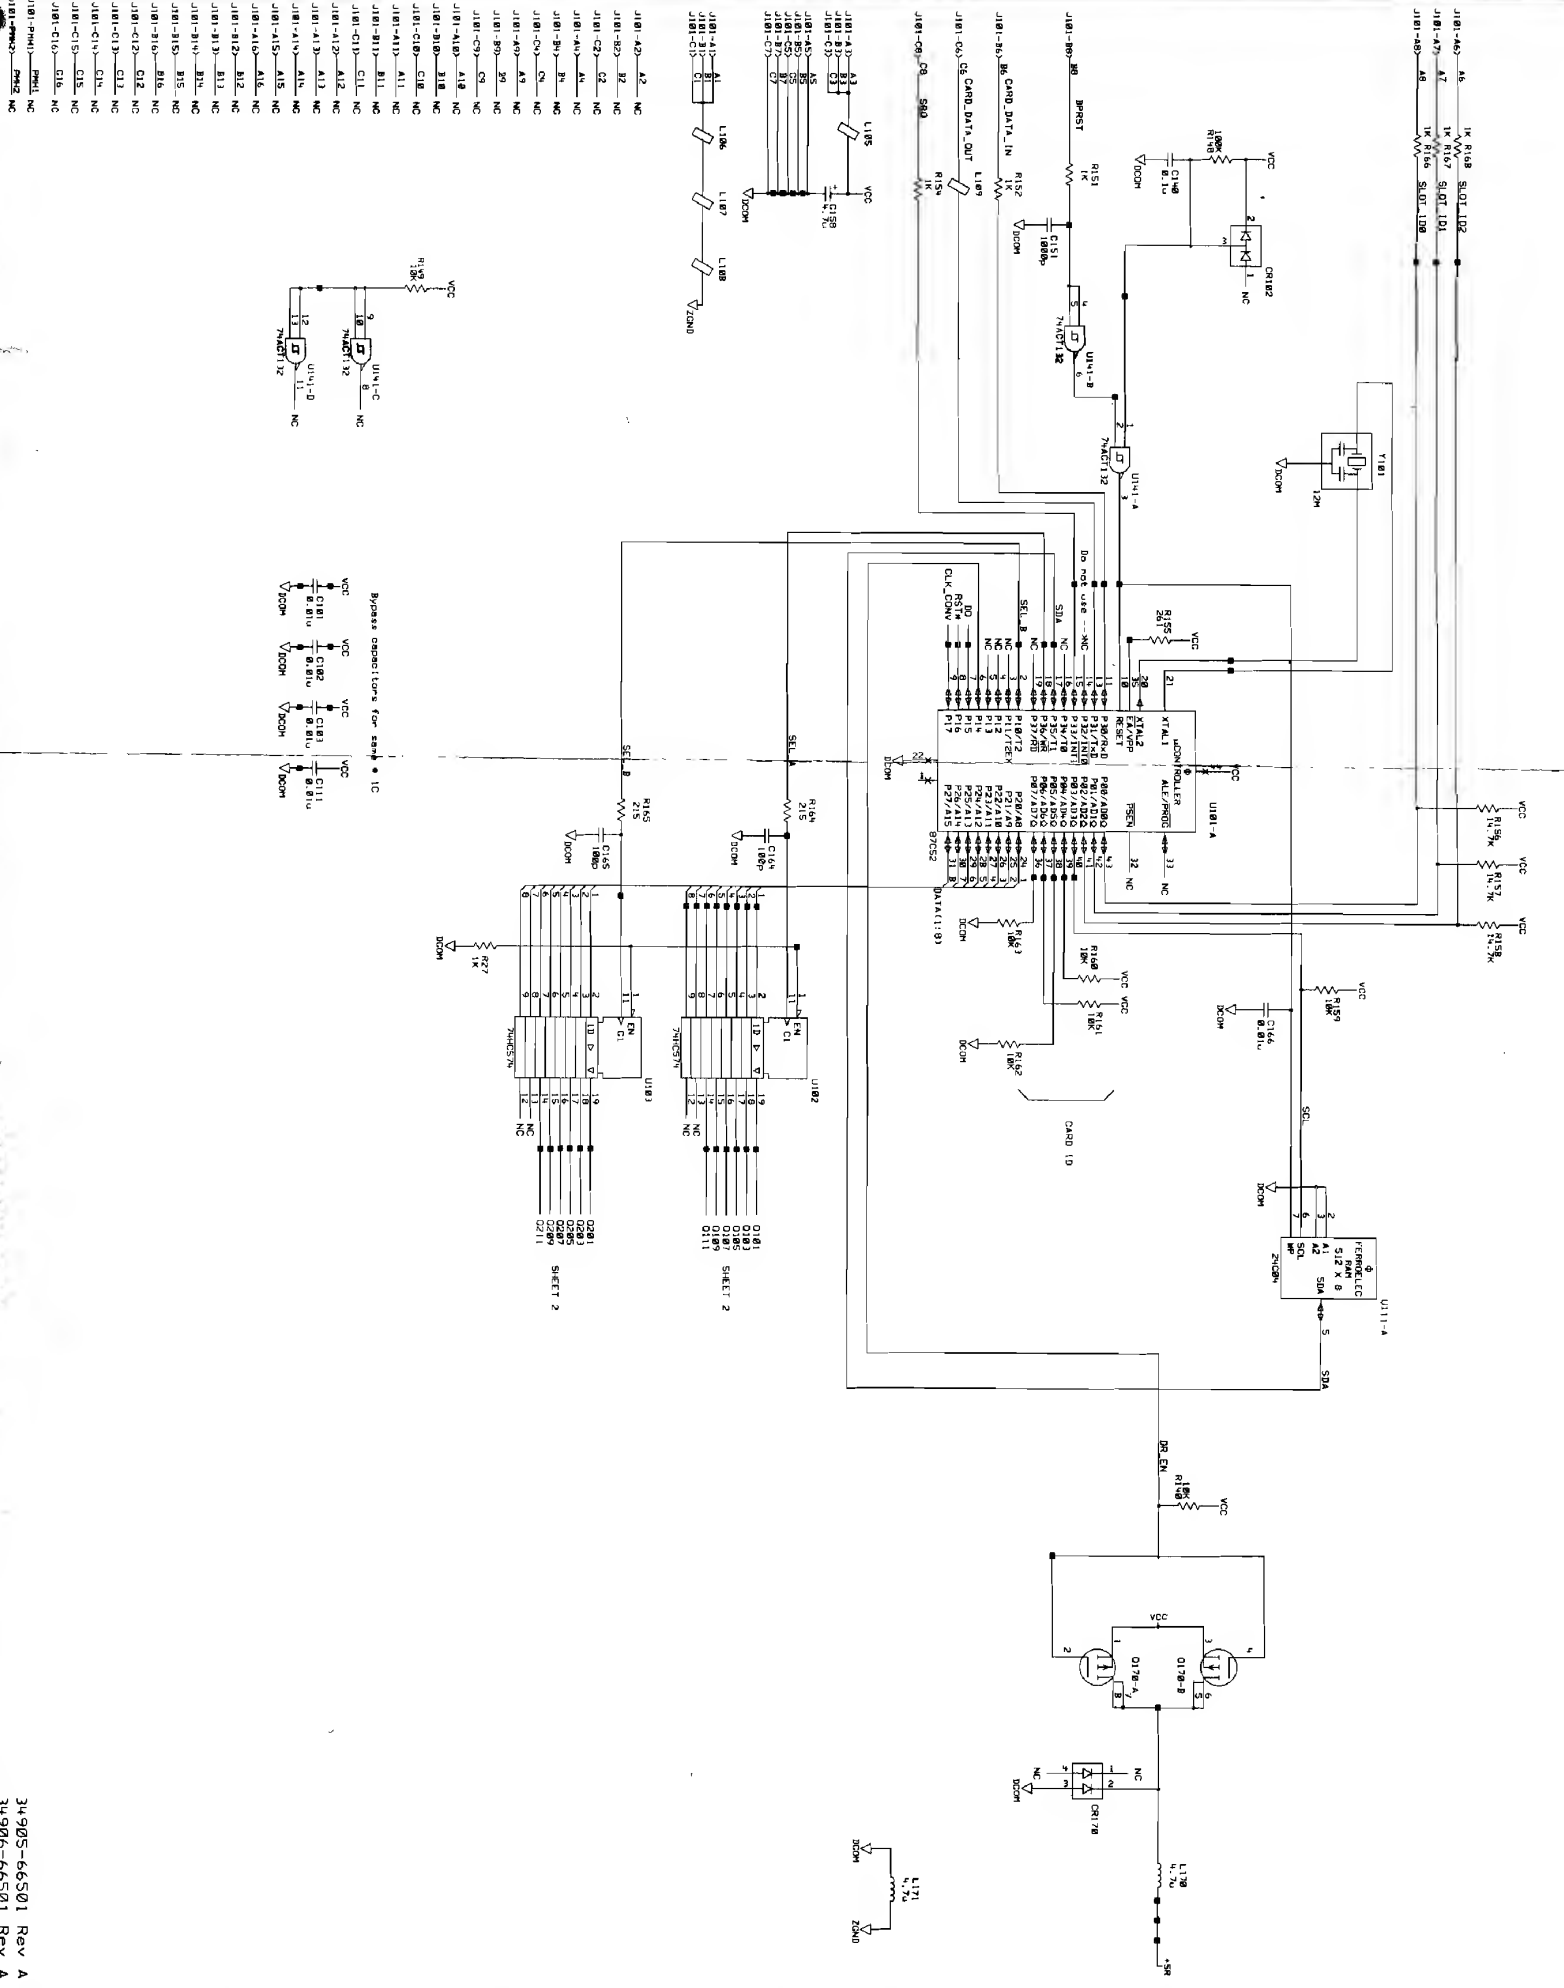

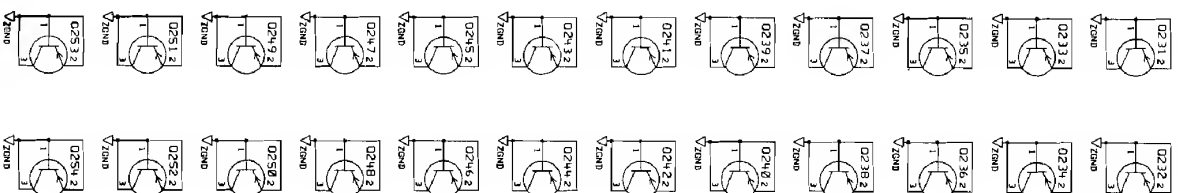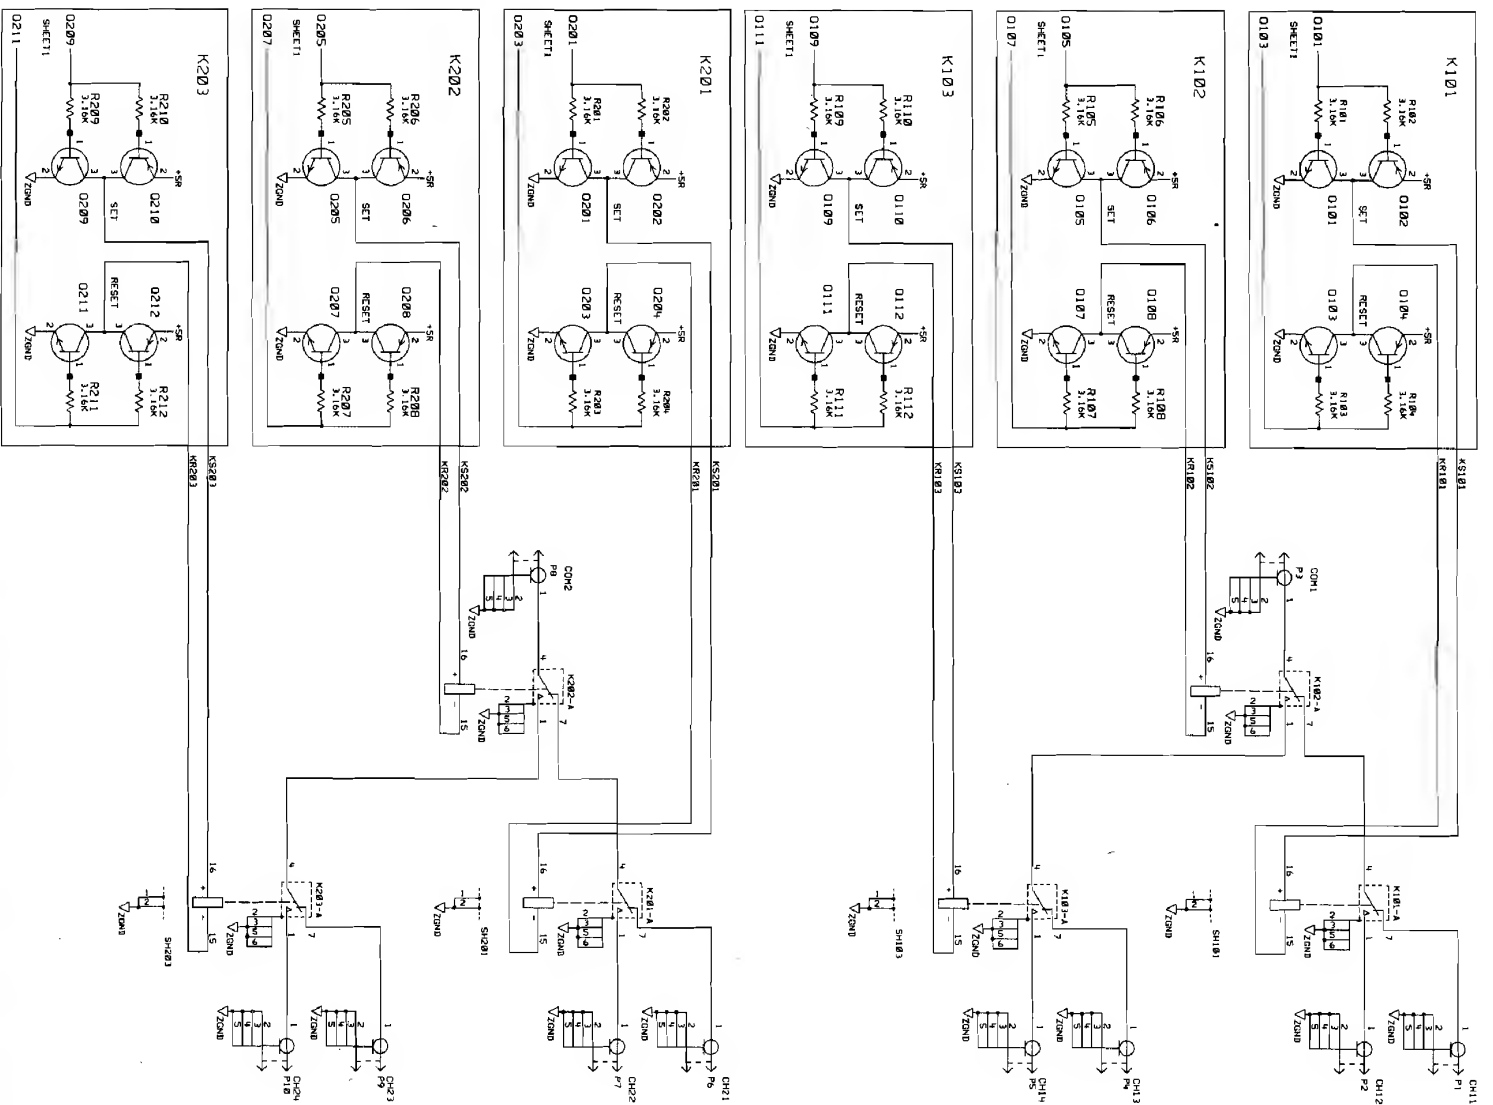

Bypass caps to be spread out among relays



VR102
VR103
VR104

P501

VR102
VR103
VR104

P101
P401
P301

U401

U402

U301

U302

RP401
RP402
RP201
RP202
RP203
RP204
RP301
RP302

CR401

CR402

Q401

Q402

CR403

CR404

Q403

Q404

CR405

CR406

Q405

Q406

CR407

CR408

Q407

Q408

CR301

CR302

Q301

Q302

CR303

CR304

Q303

Q304

CR305

CR306

Q305

Q306

CR307

CR308

Q307

Q308

RP405

RP403

R216

U206

C207

RP404

RP406

RP305

RP303

R215

U205


C206

RP304

RP306


34907-66501 Rev A


HP 34907A Multifunction Module Component Locator

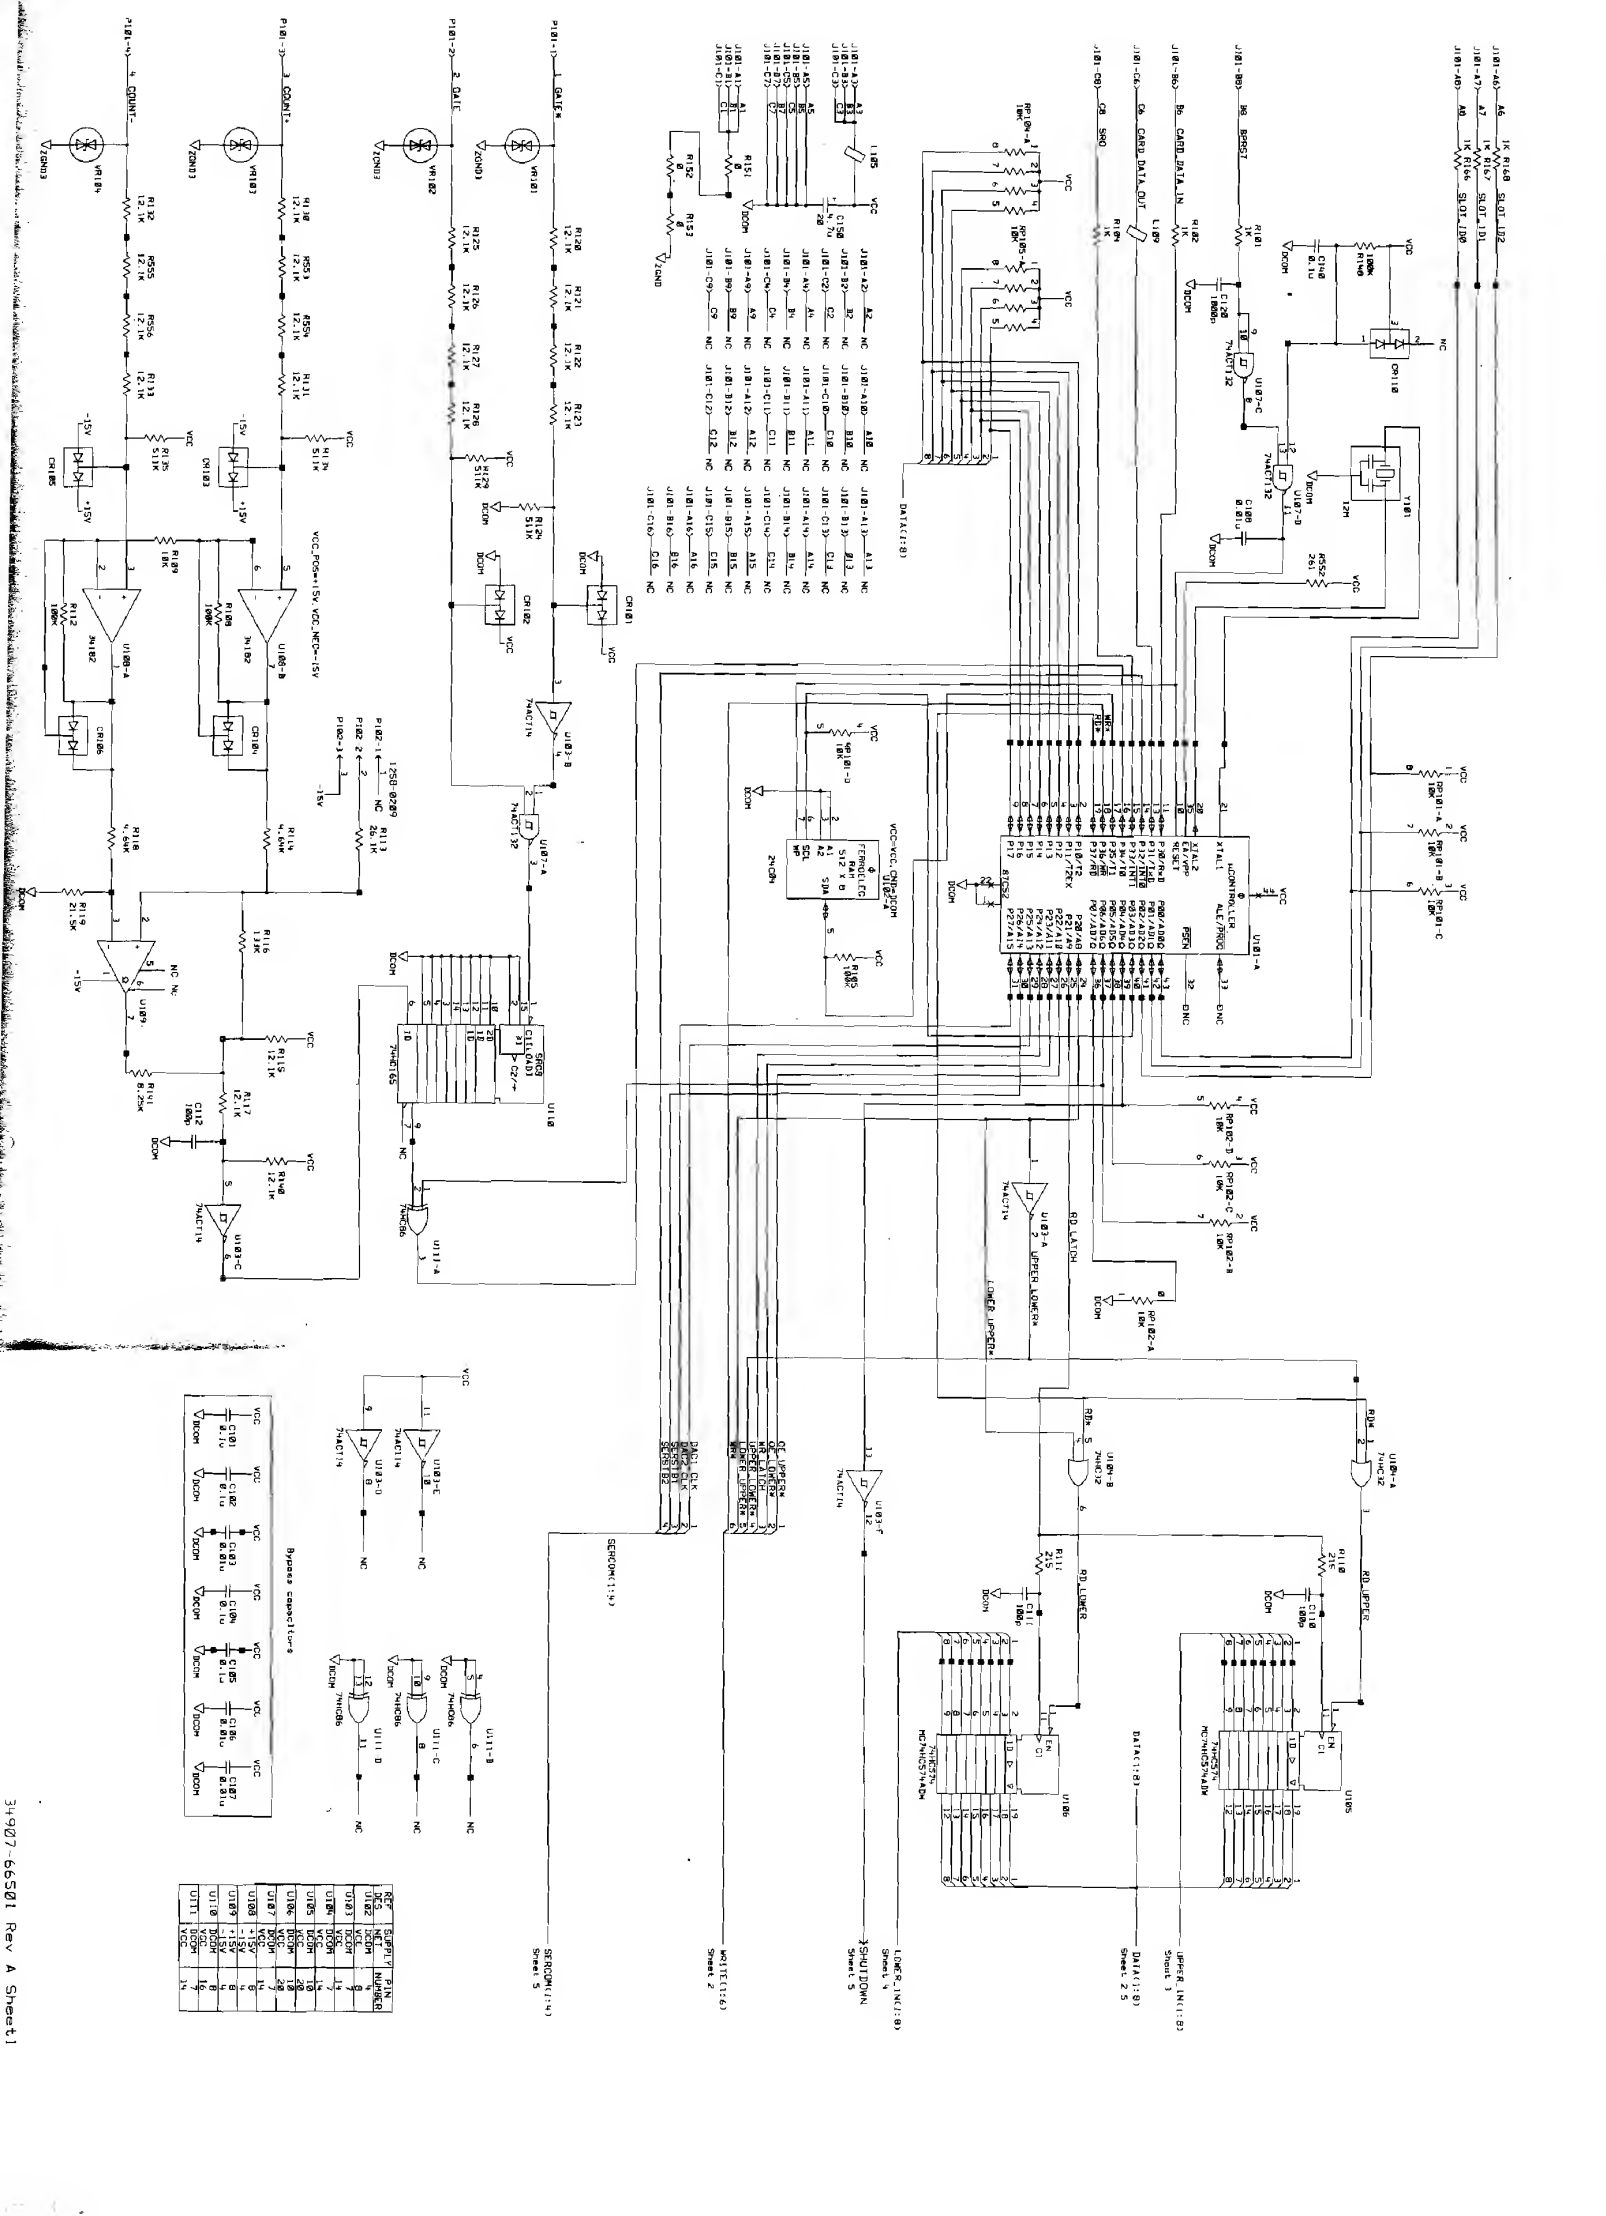





OUTPUT LATCHES & HIGH DRIVERS


REF	SUPPLY	PIN
DES	NET	NUMBER
U104	DCOM	10
U201	DCOM	10
U202	VCC	20
U203	DCOM	10
U204	VCC	20
U205	DCOM	10
U206	VCC	20
U207	DCOM	10
U208	VCC	20
U209	DCOM	10
U210	VCC	20
U211	DCOM	10
U212	VCC	20
U213	DCOM	10
U214	VCC	20
U215	DCOM	10
U216	VCC	20
U217	DCOM	10
U218	VCC	20
U219	DCOM	10
U220	VCC	20
U221	DCOM	10
U222	VCC	20
U223	DCOM	10
U224	VCC	20
U225	DCOM	10
U226	VCC	20
U227	DCOM	10
U228	VCC	20
U229	DCOM	10
U230	VCC	20
U231	DCOM	10
U232	VCC	20
U233	DCOM	10
U234	VCC	20
U235	DCOM	10
U236	VCC	20
U237	DCOM	10
U238	VCC	20
U239	DCOM	10
U240	VCC	20
U241	DCOM	10
U242	VCC	20
U243	DCOM	10
U244	VCC	20
U245	DCOM	10
U246	VCC	20
U247	DCOM	10
U248	VCC	20
U249	DCOM	10
U250	VCC	20
U251	DCOM	10
U252	VCC	20
U253	DCOM	10
U254	VCC	20
U255	DCOM	10
U256	VCC	20
U257	DCOM	10
U258	VCC	20
U259	DCOM	10
U260	VCC	20
U261	DCOM	10
U262	VCC	20
U263	DCOM	10
U264	VCC	20
U265	DCOM	10
U266	VCC	20
U267	DCOM	10
U268	VCC	20
U269	DCOM	10
U270	VCC	20
U271	DCOM	10
U272	VCC	20
U273	DCOM	10
U274	VCC	20
U275	DCOM	10
U276	VCC	20
U277	DCOM	10
U278	VCC	20
U279	DCOM	10
U280	VCC	20
U281	DCOM	10
U282	VCC	20
U283	DCOM	10
U284	VCC	20
U285	DCOM	10
U286	VCC	20
U287	DCOM	10
U288	VCC	20
U289	DCOM	10
U290	VCC	20
U291	DCOM	10
U292	VCC	20
U293	DCOM	10
U294	VCC	20
U295	DCOM	10
U296	VCC	20
U297	DCOM	10
U298	VCC	20
U299	DCOM	10
U300	VCC	20

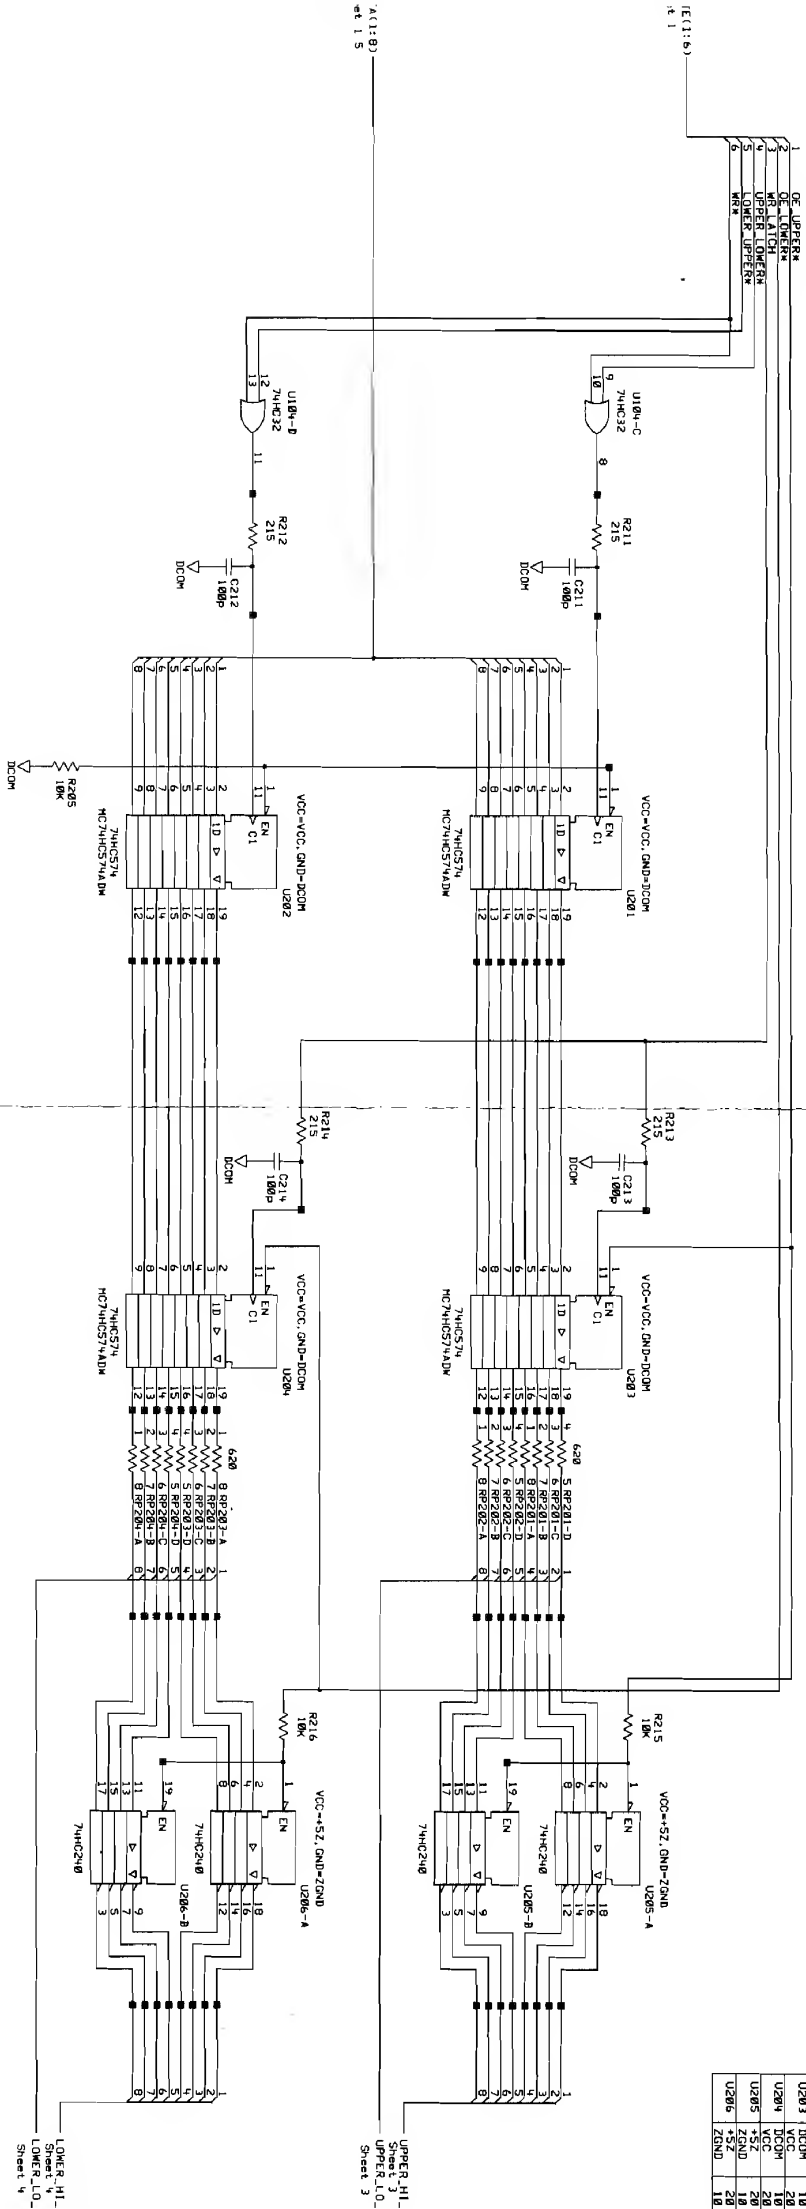


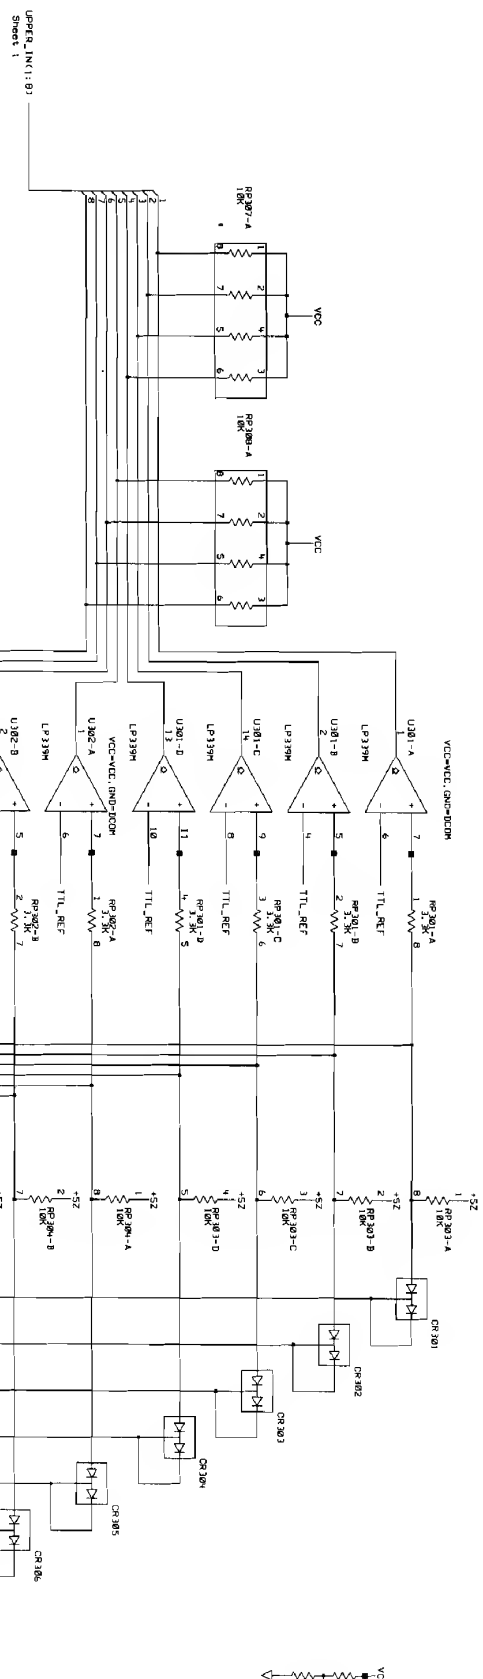





REF	SUPPLY	PIN
U101-A	VCC	1
U101-B	VCC	1
U101-C	VCC	1
U101-D	VCC	1
U102-A	VCC	1
U102-B	VCC	1
U102-C	VCC	1
U102-D	VCC	1
U103-A	VCC	1
U103-B	VCC	1
U103-C	VCC	1
U103-D	VCC	1
U104-A	VCC	1
U104-B	VCC	1
U104-C	VCC	1
U104-D	VCC	1
U105-A	VCC	1

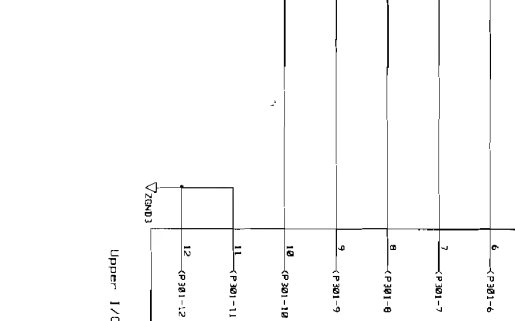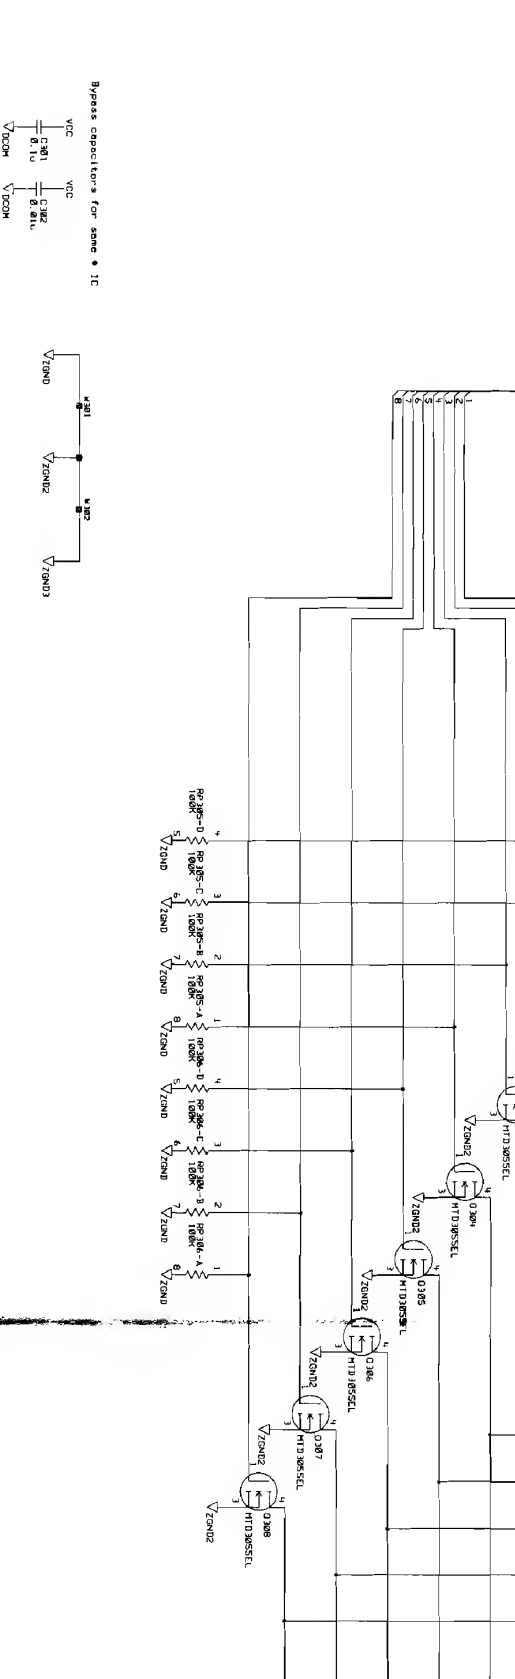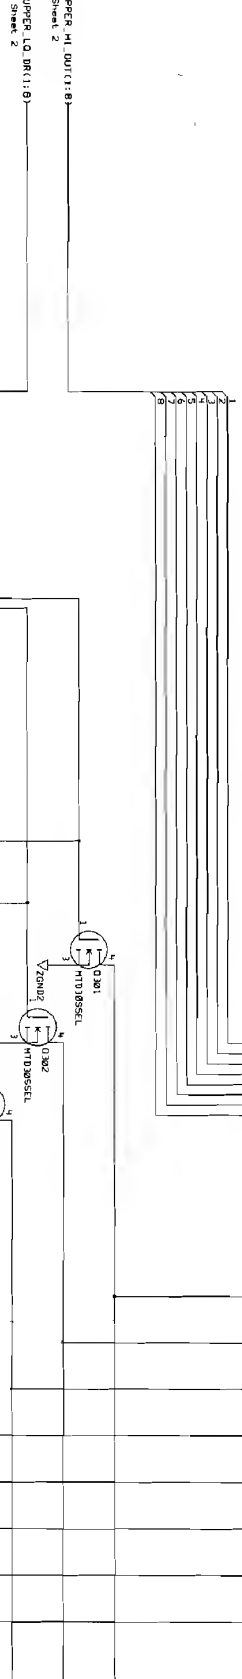

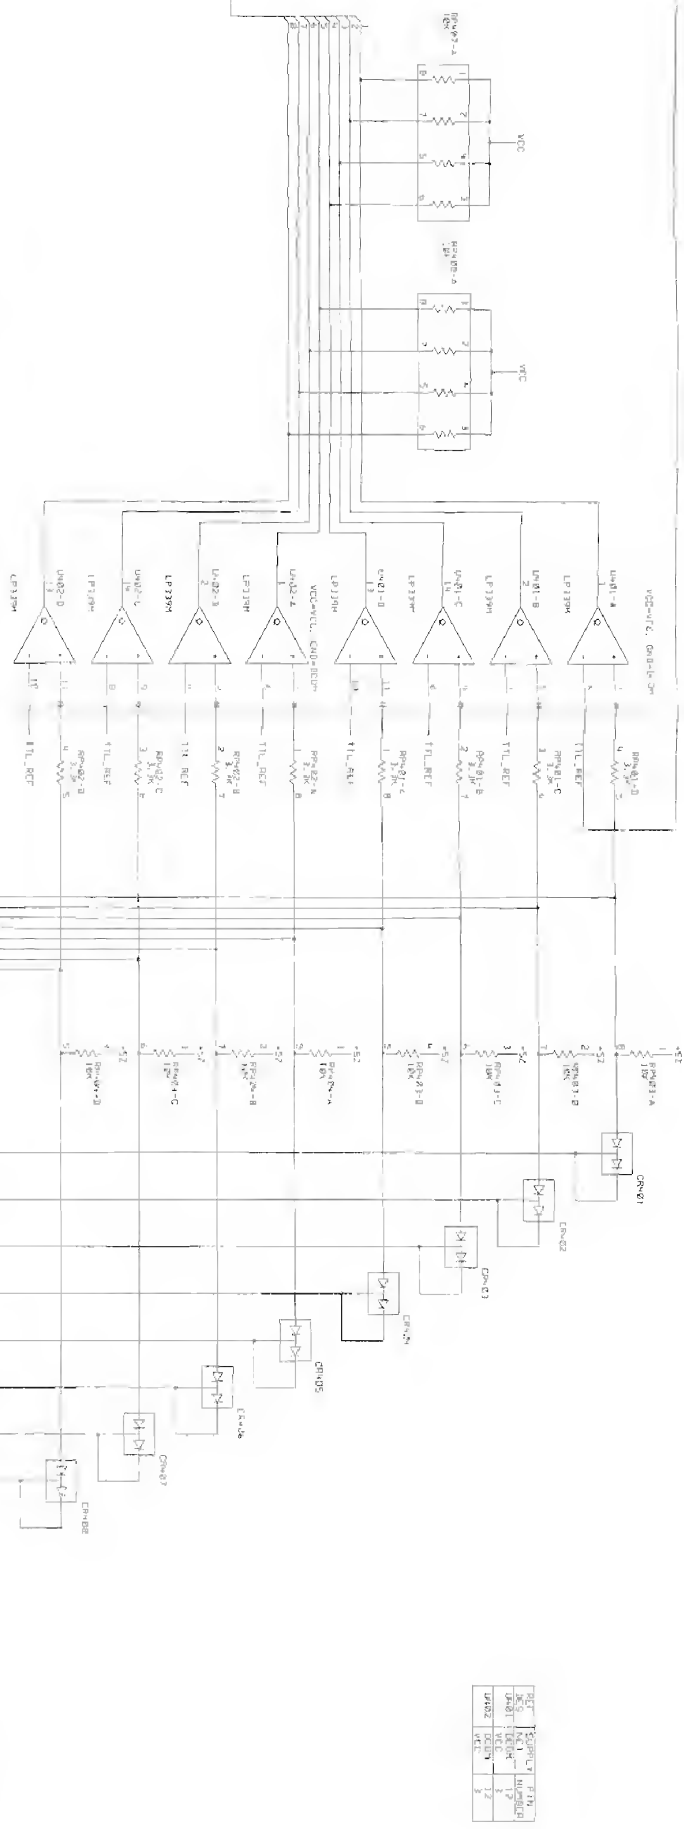


REF	DESCRIPTION	PIN
1	0.000-20	1
2	0.000-10	2
3	0.000-5	3
4	0.000-2.5	4
5	0.000-1.25	5

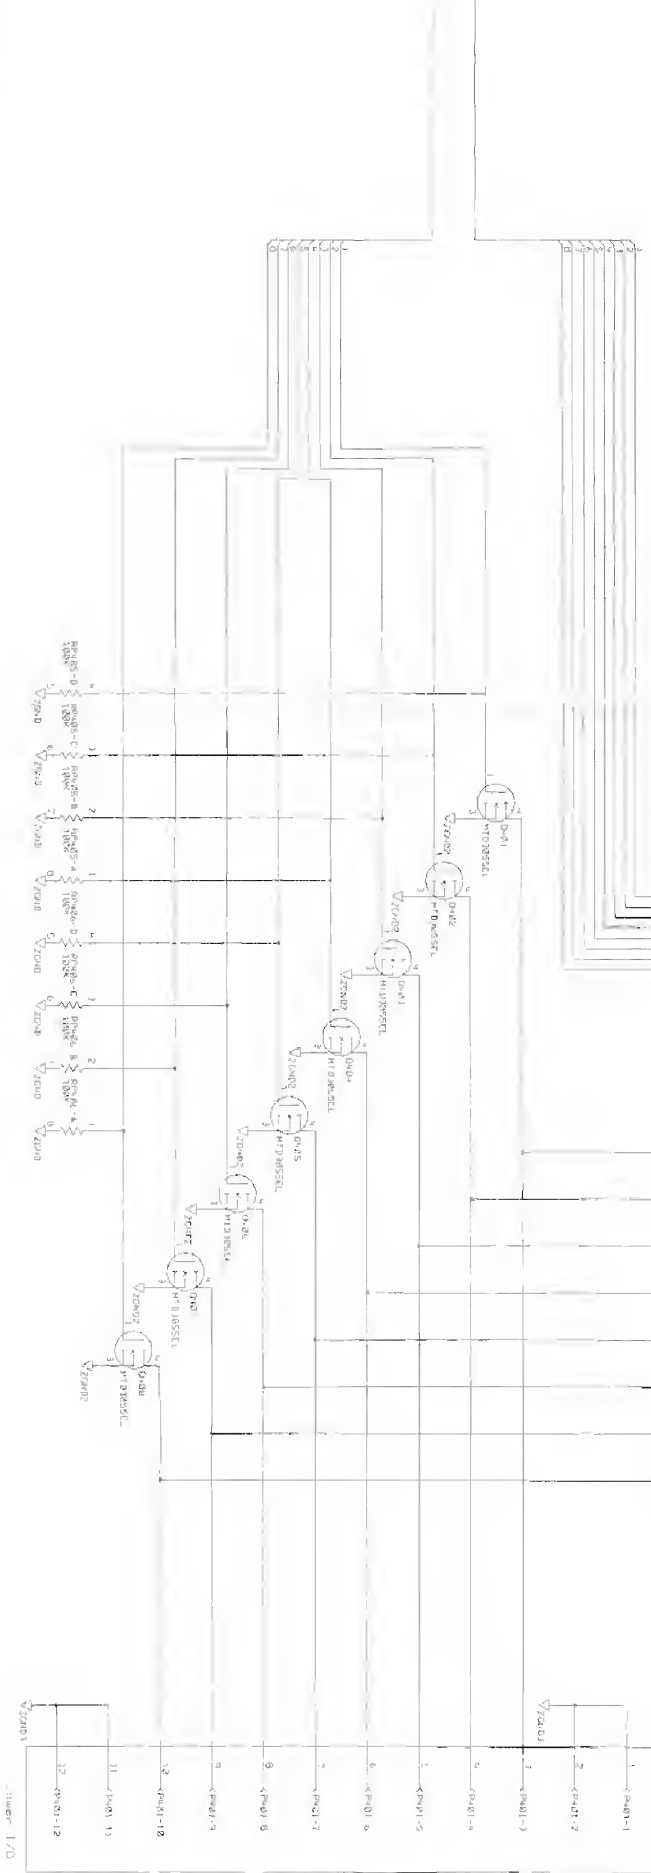

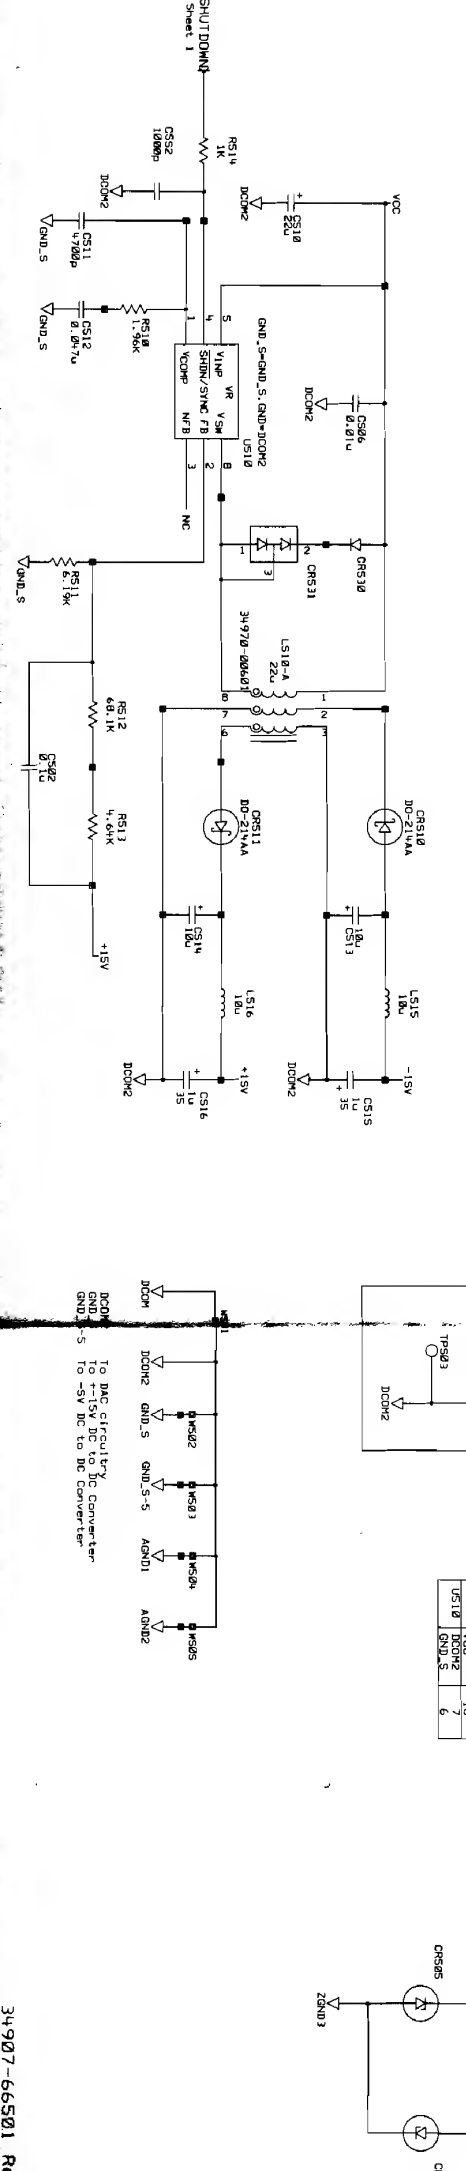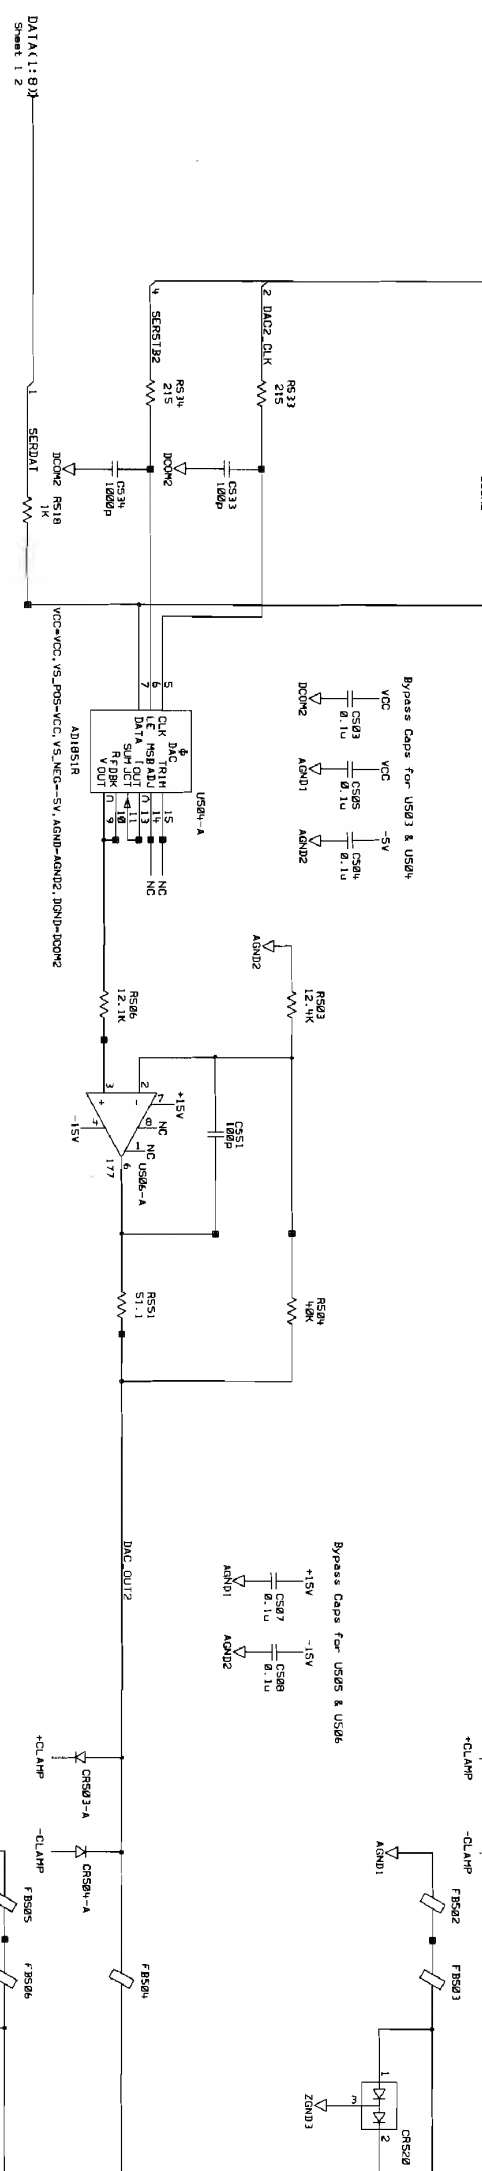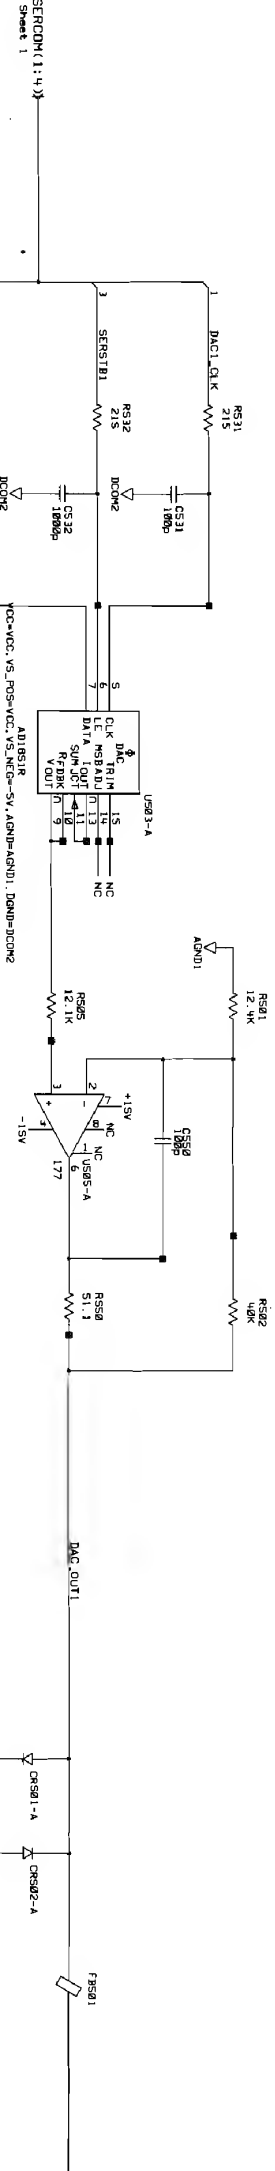




REF	NET	SUPPLY	PTN
US03	US03	VCC	1
US04	US04	VCC	2
US05	US05	VCC	3
US06	US06	VCC	4
US07	US07	VCC	5
US08	US08	VCC	6
US09	US09	VCC	7
US10	US10	VCC	8
US11	US11	VCC	9
US12	US12	VCC	10
US13	US13	VCC	11
US14	US14	VCC	12
US15	US15	VCC	13
US16	US16	VCC	14
US17	US17	VCC	15
US18	US18	VCC	16
US19	US19	VCC	17
US20	US20	VCC	18
US21	US21	VCC	19
US22	US22	VCC	20
US23	US23	VCC	21
US24	US24	VCC	22
US25	US25	VCC	23
US26	US26	VCC	24
US27	US27	VCC	25
US28	US28	VCC	26
US29	US29	VCC	27
US30	US30	VCC	28
US31	US31	VCC	29
US32	US32	VCC	30
US33	US33	VCC	31
US34	US34	VCC	32
US35	US35	VCC	33
US36	US36	VCC	34
US37	US37	VCC	35
US38	US38	VCC	36
US39	US39	VCC	37
US40	US40	VCC	38
US41	US41	VCC	39
US42	US42	VCC	40
US43	US43	VCC	41
US44	US44	VCC	42
US45	US45	VCC	43
US46	US46	VCC	44
US47	US47	VCC	45
US48	US48	VCC	46
US49	US49	VCC	47
US50	US50	VCC	48
US51	US51	VCC	49
US52	US52	VCC	50
US53	US53	VCC	51
US54	US54	VCC	52
US55	US55	VCC	53
US56	US56	VCC	54
US57	US57	VCC	55
US58	US58	VCC	56
US59	US59	VCC	57
US60	US60	VCC	58
US61	US61	VCC	59
US62	US62	VCC	60
US63	US63	VCC	61
US64	US64	VCC	62
US65	US65	VCC	63
US66	US66	VCC	64
US67	US67	VCC	65
US68	US68	VCC	66
US69	US69	VCC	67
US70	US70	VCC	68
US71	US71	VCC	69
US72	US72	VCC	70
US73	US73	VCC	71
US74	US74	VCC	72
US75	US75	VCC	73
US76	US76	VCC	74
US77	US77	VCC	75
US78	US78	VCC	76
US79	US79	VCC	77
US80	US80	VCC	78
US81	US81	VCC	79
US82	US82	VCC	80
US83	US83	VCC	81
US84	US84	VCC	82
US85	US85	VCC	83
US86	US86	VCC	84
US87	US87	VCC	85
US88	US88	VCC	86
US89	US89	VCC	87
US90	US90	VCC	88
US91	US91	VCC	89
US92	US92	VCC	90
US93	US93	VCC	91
US94	US94	VCC	92
US95	US95	VCC	93
US96	US96	VCC	94
US97	US97	VCC	95
US98	US98	VCC	96
US99	US99	VCC	97
US100	US100	VCC	98
US101	US101	VCC	99
US102	US102	VCC	100

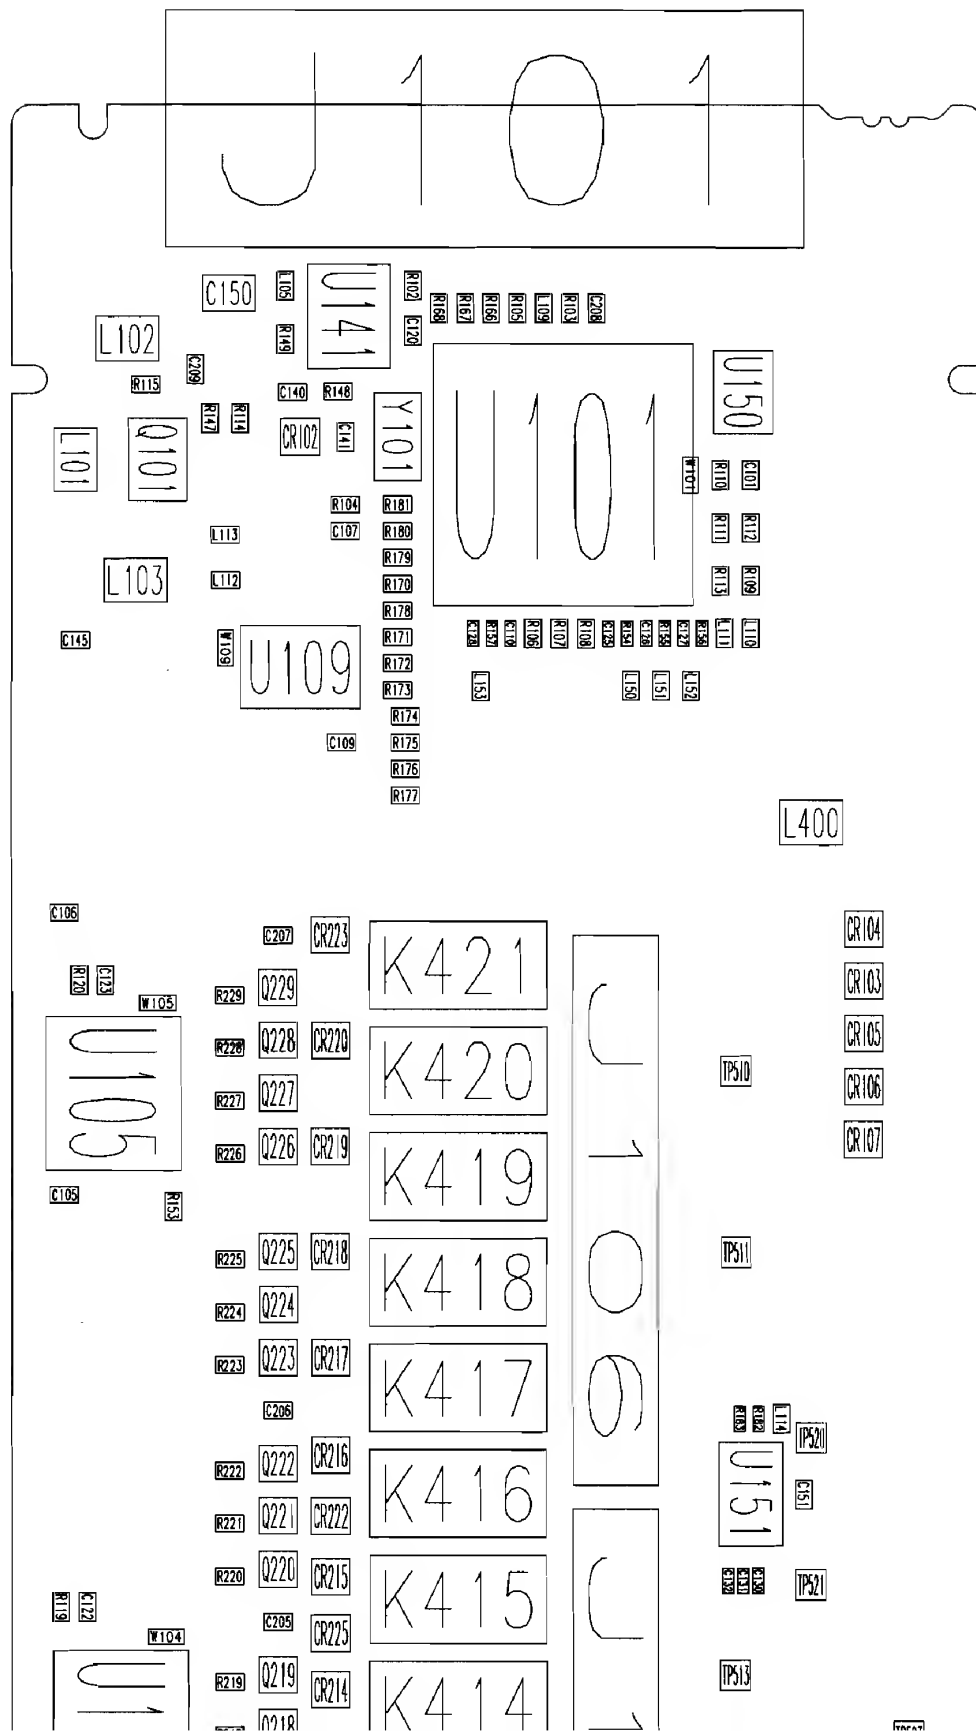

34908-66501 Rev B

HP 34908A 40-Channel Multiplexer Component Locator

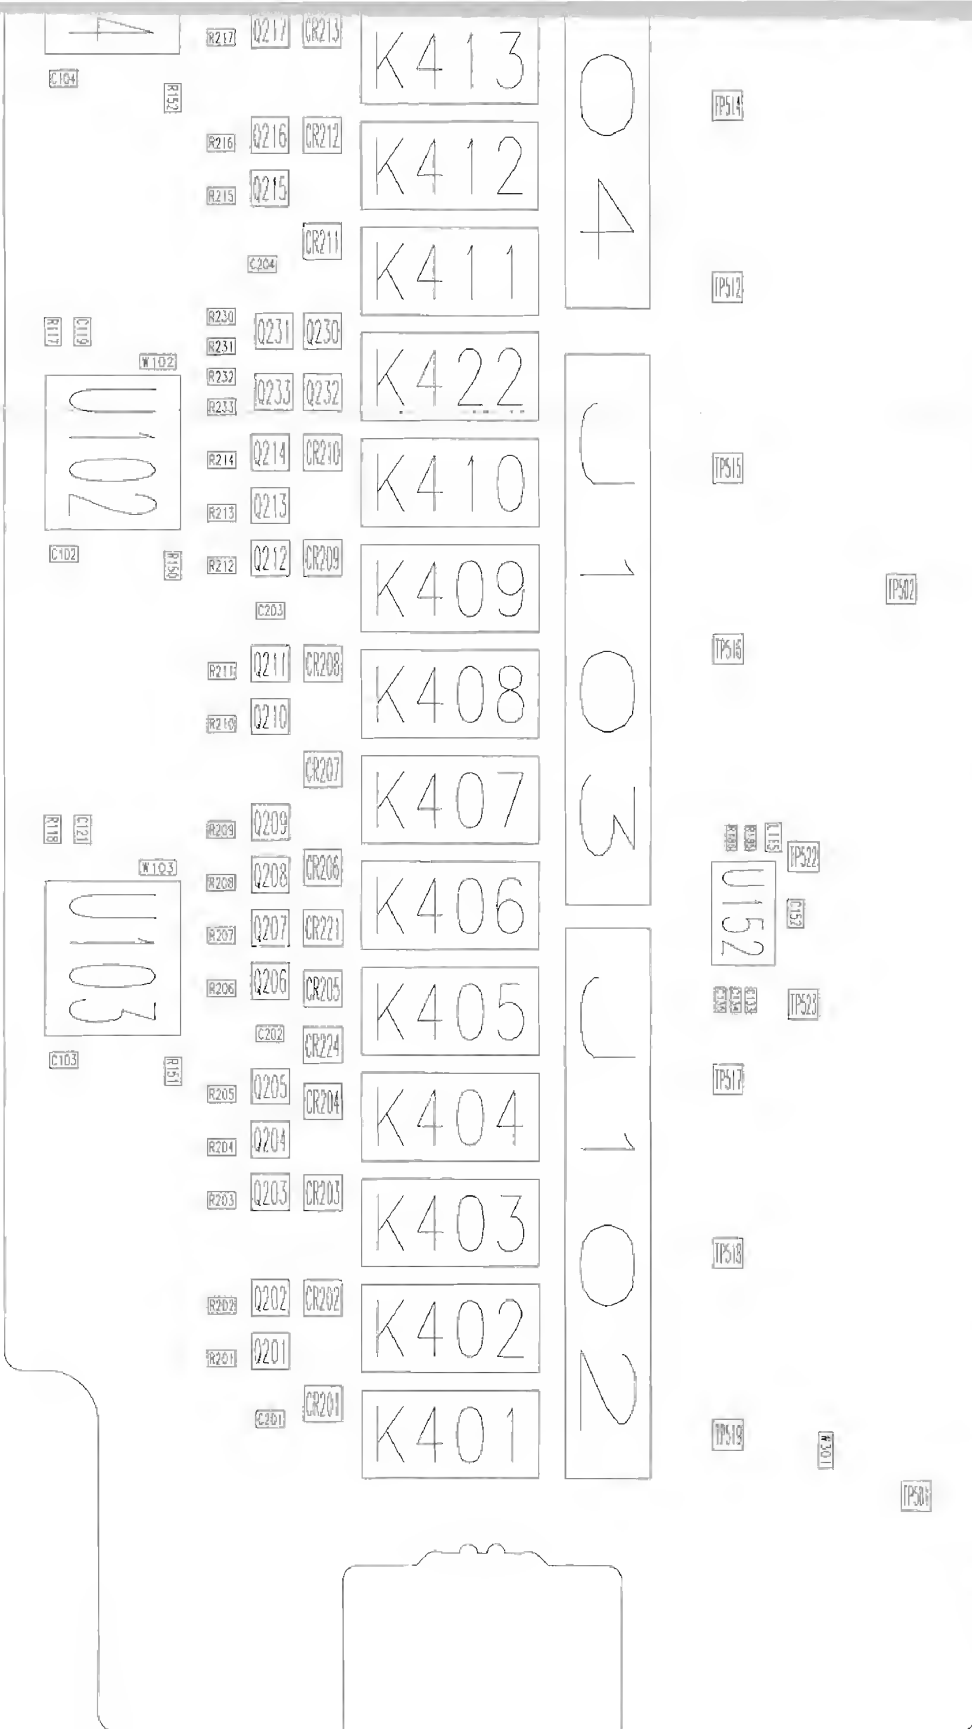

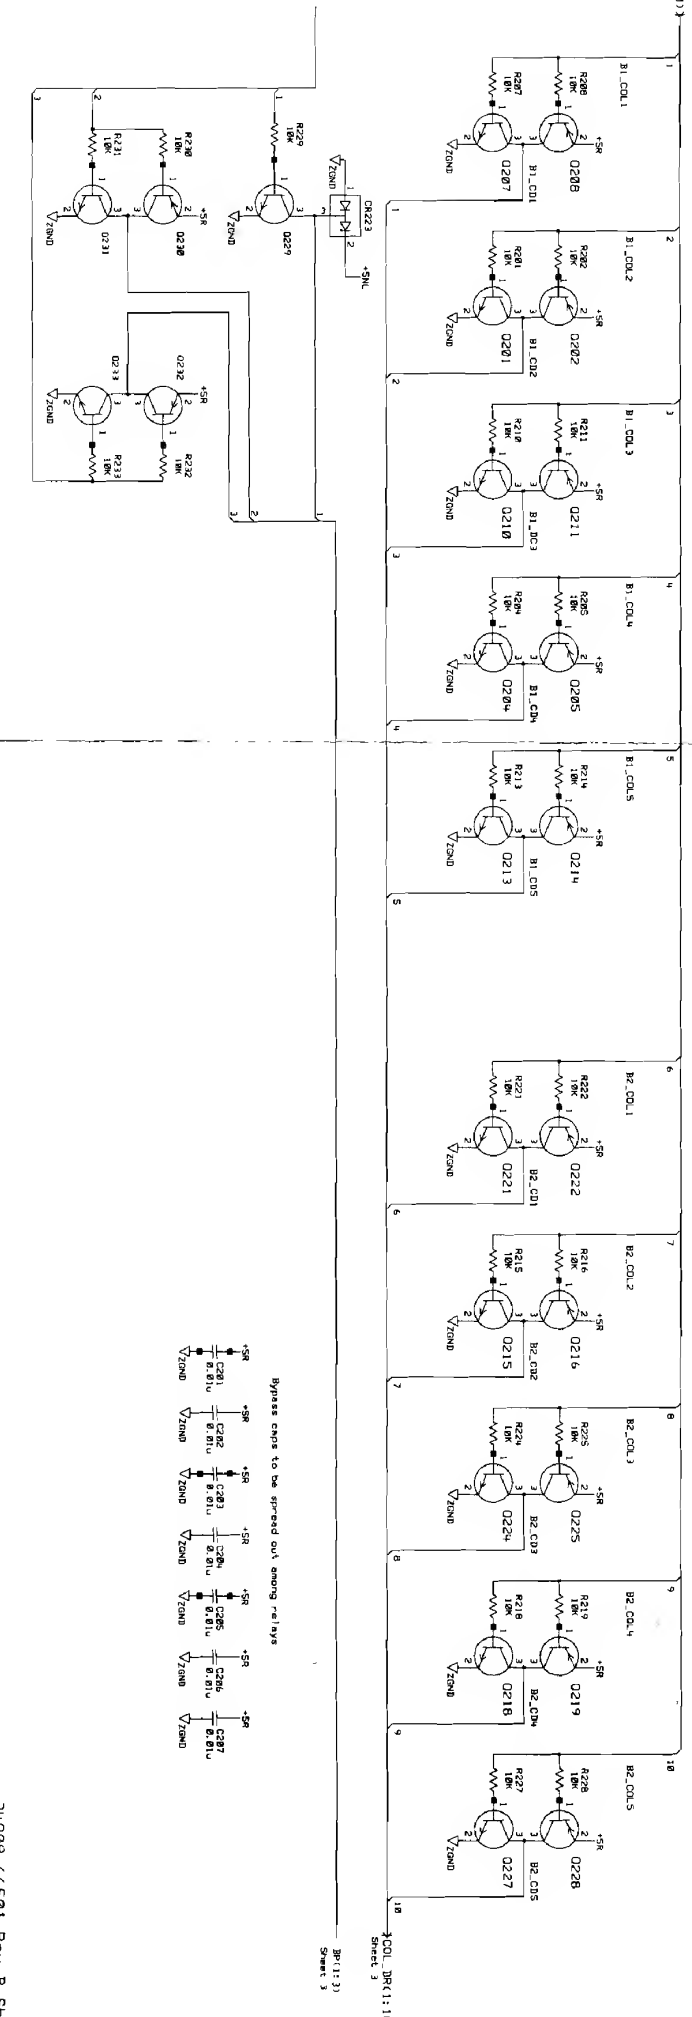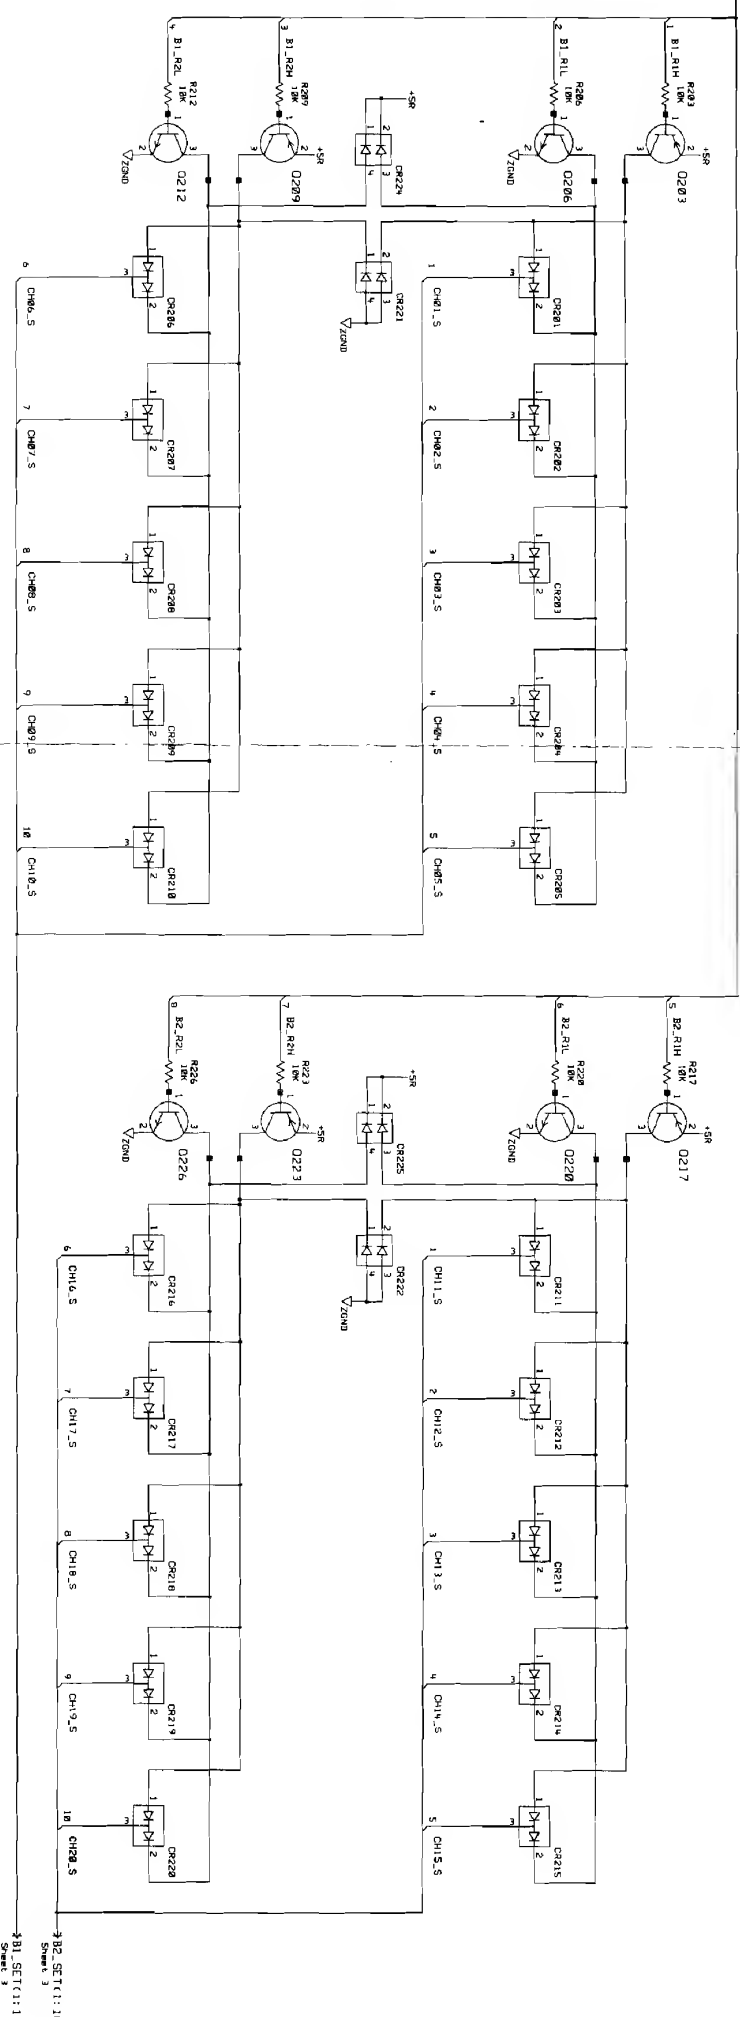

Bypass caps to be spread out among columns

+5V
C281 10k
VZND

+5V
C282 10k
VZND




+5V
C283 10k
VZND

+5V
C284 10k
VZND


+5V
C285 10k
VZND

+5V
C286 10k
VZND

+5V
C287 10k
VZND

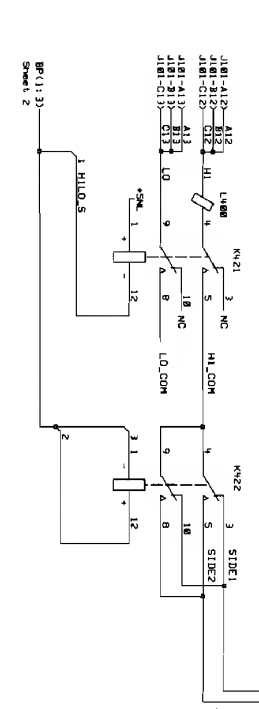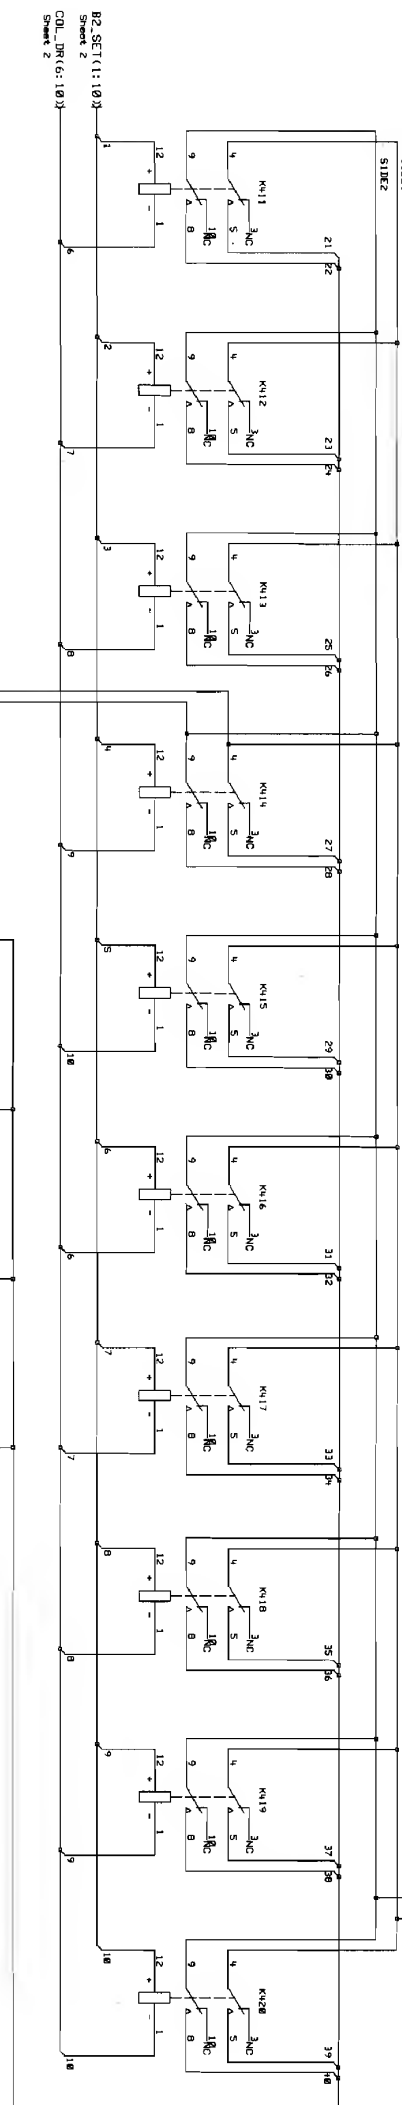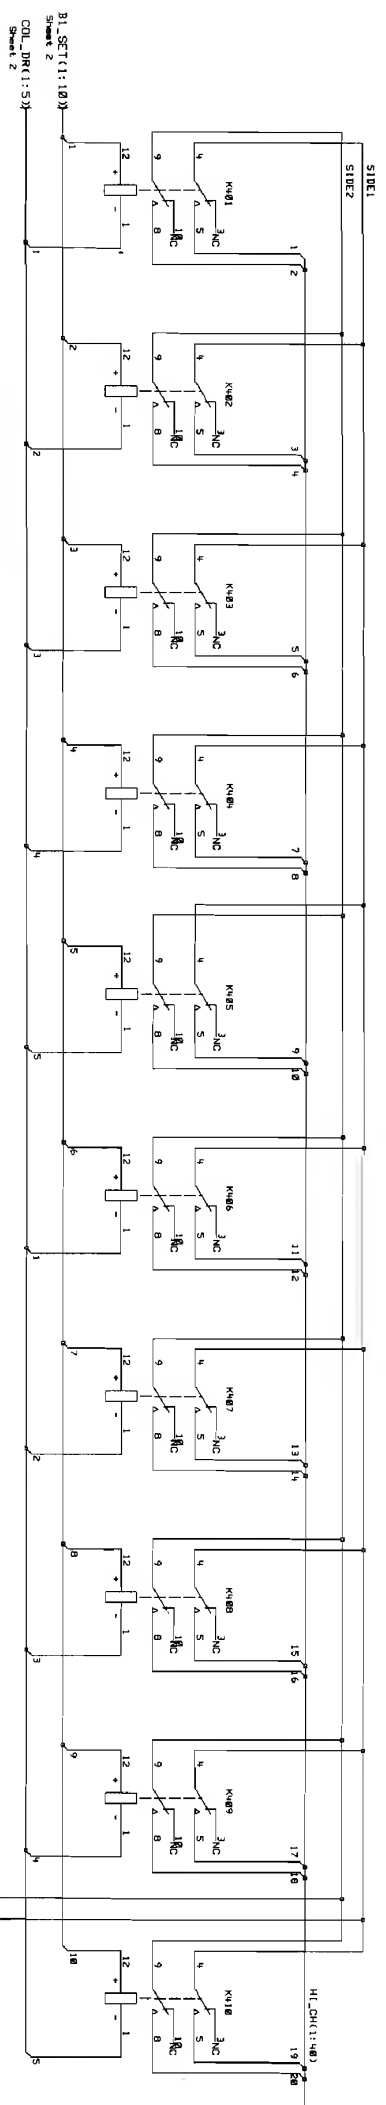



RELAY SCHEMATIC (BOTTOM VIEW)

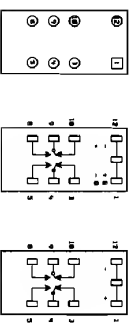

68NU-2-Y-DC3

1. CH01 1 -> J102-1	11. CH06 1 -> J103-1	21. CH11 1 -> J104-1	31. CH16 1 -> J105-1
2. CH01 2 -> J102-2	12. CH06 2 -> J103-2	22. CH11 2 -> J104-2	32. CH16 2 -> J105-2
3. CH02 3 -> J102-3	13. CH07 3 -> J103-3	23. CH12 3 -> J104-3	33. CH17 3 -> J105-3
4. CH02 4 -> J102-4	14. CH07 4 -> J103-4	24. CH12 4 -> J104-4	34. CH17 4 -> J105-4
5. CH03 5 -> J102-5	15. CH08 5 -> J103-5	25. CH13 5 -> J104-5	35. CH18 5 -> J105-5
6. CH03 6 -> J102-6	16. CH08 6 -> J103-6	26. CH13 6 -> J104-6	36. CH18 6 -> J105-6
7. CH04 7 -> J102-7	17. CH09 7 -> J103-7	27. CH14 7 -> J104-7	37. CH19 7 -> J105-7
8. CH04 8 -> J102-8	18. CH09 8 -> J103-8	28. CH14 8 -> J104-8	38. CH19 8 -> J105-8
9. CH05 9 -> J102-9	19. CH10 9 -> J103-9	29. CH15 9 -> J104-9	39. CH20 9 -> J105-9
10. CH05 10 -> J102-10	20. CH10 10 -> J103-10	30. CH15 10 -> J104-10	40. CH20 10 -> J105-10
LO COM 11 -> J102-11	LO COM 11 -> J103-11	LO COM 11 -> J104-11	LO COM 11 -> J105-11
LO COM 12 -> J102-12	LO COM 12 -> J103-12	LO COM 12 -> J104-12	LO COM 12 -> J105-12

USER CONNECTORS

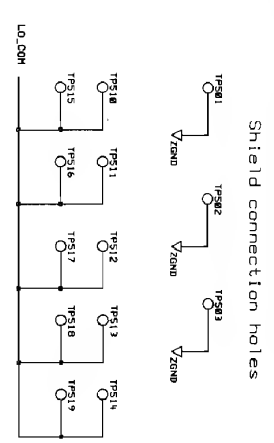



Quick Reference Guide

SCPI Command Summary

The following conventions are used for SCPI command syntax for remote interface programming:

- Square brackets ([]) indicate optional keywords or parameters.
- Braces ({ }) enclose parameter choices within a command string.
- Triangle brackets (< >) enclose parameters for which you must substitute a value.
- A vertical bar (|) separates multiple parameter choices.

Rules for Using a Channel List

Many of the SCPI commands for the 34970A include a *scan_list* or *ch_list* parameter which allow you to specify one or more channels. The channel number has the form (@*scc*), where *s* is the slot number (100, 200, or 300) and *cc* is the channel number. You can specify a single channel, multiple channels, or a range of channels as shown below.

- The following command configures a scan list to include only channel 10 on the module in slot 300.

```
ROUT:SCAN (@310)
```

- The following command configures a scan list to include multiple channels on the module in slot 200. The scan list now contains only channels 10, 12, and 15 (*the scan list is redefined each time you send a new ROUTe:SCAN command*).

```
ROUT:SCAN (@210,212,215)
```

- The following command configures a scan list to include a range of channels. When you specify a range of channels, the range *may* contain invalid channels (they are ignored), but the first and last channel in the range must be valid. The scan list now contains channels 5 through 10 (slot 100) and channel 15 (slot 200).

```
ROUT:SCAN (@105:110,215)
```

Scan Measurement Commands

(see page 226 in the User's Guide)

S MEASure
:TEMPerature? {**TCouple**|RTD|FRTD|THERmistor|DEF}
[, {<type>|DEF}[, 1[, {<resolution>|MIN|MAX|DEF}]] , (@<scan_list>)
:VOLTage:DC? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:VOLTage:AC? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:RESistance? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:FRESistance? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:CURRent:DC? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:CURRent:AC? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:FREQuency? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:PERiod? [{<range>|**AUTO**|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF}] ,] (@<scan_list>)
:DIGital:BYTE? (@<scan_list>)
:TOTAlize? {**READ**|RRESet} , (@<scan_list>)

Monitor Commands

(see page 237 in the User's Guide)

ROUTE
:MONitor (@<channel>)
:MONitor?

ROUTE
:MONitor:STATe (**OFF**|ON)
:MONitor:STATe?

ROUTE:MONitor:DATA?

Scan Statistics Commands

(see page 233 in the User's Guide)

CALCulate
:AVERage:MINimum? [{@<ch_list>}]
:AVERage:MINimum:TIME? [{@<ch_list>}]
:AVERage:MAXimum? [{@<ch_list>}]
:AVERage:MAXimum:TIME? [{@<ch_list>}]
:AVERage:AVERage? [{@<ch_list>}]
:AVERage:PTPeak? [{@<ch_list>}]
:AVERage:COUNt? [{@<ch_list>}]
:AVERage:CLEar [{@<ch_list>}]

DATA:LAST? [<num_rds> ,] [(@<channel>)]

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Scan Configuration Commands

(see page 226 in the User's Guide)

```

ROUTe
S :SCAN (@<scan_list>)
    :SCAN?
    :SCAN:SIZE?

G TRIGger
    :SOURce {BUS|IMMediate|EXTeRnal|ALARm1|ALARm2|ALARm3|ALARm4|TIME}
    :SOURce?

G TRIGger
    :TIMer {<seconds>|MIN|MAX}
    :TIMer?

G TRIGger
    :COUNT {<count>|MIN|MAX|INFIinity}
    :COUNT?

ROUTe
    :CHANnel:DElay <seconds>[, (@<ch_list>)]
    :CHANnel:DElay? [{@<ch_list>}]
    :CHANnel:DElay:AUTO {OFF|ON}[, (@<ch_list>)]
    :CHANnel:DElay:AUTO? [{@<ch_list>}]

G FORMat
    :READing:ALARm {OFF|ON}
    :READing:ALARm?
    :READing:CHANnel {OFF|ON}
    :READing:CHANnel?
    :READing:TIME {OFF|ON}
    :READing:TIME?
    :READing:UNIT {OFF|ON}
    :READing:UNIT?

G FORMat
    :READing:TIME:TYPE {ABSolute|RELative}
    :READing:TIME:TYPE?

ABORT

INITiate

READ?

```

Scan Memory Commands

(see page 235 in the User's Guide)

```

DATA:POINts?

DATA:REMOve? <num_rdg>

SYSTem:TIME:SCAN?

FETCh?


R? [<max_count>]

```

- S** This command redefines the scan list when executed.
- G** This command applies to all channels in the instrument (Global setting). Default parameters are shown in **bold**.

Scanning With an External Instrument

(see page 239 in the User's Guide)

S ROUTe

:SCAN?
:SCAN:SIZE?

G TRIGger
:SOURce {BUS|IMMediate|EXtErnal|**TIMer**}
:SOURce?

G TRIGger
:TIMer {<seconds>|**MIN**|MAX}
:TIMer?

G TRIGger
:COUNT {<count>|MIN|MAX|**INfinity**}
:COUNT?

ROUTe
:CHANnel:DElay <seconds>[, (@<ch_list>)]
:CHANnel:DElay? [{@<ch_list>}]

G ROUTe
:CHANnel:ADVance:SOURce {**EXtErnal**|BUS|IMMediate}
:CHANnel:ADVance:SOURce?

ROUTe
:CHANnel:FWIRE {OFF|ON}[, (@<ch_list>)]
:CHANnel:FWIRE? [{@<ch_list>}]

G INSTRument
:DMM {OFF|ON}
:DMM?
:DMM:INSTalled?

S This command redefines the scan list when executed.

G This command applies to all channels in the instrument (Global setting).
Default parameters are shown in **bold**.

Temperature Configuration Commands

(see page 219 in the User's Guide)

```

S CONFigure
    :TEMPerature {TCouple|RTD|FRTD|THERmistor|DEF}
    , {<type>|DEF}{,1{,<resolution>|MIN|MAX|DEF}}}, {<@<scan_list>}
CONFigure? [{<@<ch_list>}]

UNIT
    :TEMPerature {C|F|K}{,<@<ch_list>}}
    :TEMPerature? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :TYPE {TCouple|RTD|FRTD|THERmistor|DEF}{,<@<ch_list>}}
    :TYPE? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :TCouple:TYPE {B|E|J|K|N|R|S|T}{,<@<ch_list>}}
    :TCouple:TYPE? [{<@<ch_list>}]
    :TCouple:CHECK {OFF|ON}{,<@<ch_list>}}
    :TCouple:CHECK? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :TCouple:RJUNCTION:TYPE {INTernal|EXternal|FIXed}{,<@<ch_list>}}
    :TCouple:RJUNCTION:TYPE? [{<@<ch_list>}]
    :TCouple:RJUNCTION {<temperature>|MIN|MAX}{,<@<ch_list>}}
    :TCouple:RJUNCTION? [{<@<ch_list>}]

[SENSe:]TEMPerature:RJUNCTION? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :RTD:TYPE {85|91}{,<@<ch_list>}}
    :RTD:TYPE? [{<@<ch_list>}]
    :RTD:RESistance[:REfERENCE] <reference>{,<@<ch_list>}}
    :RTD:RESistance[:REfERENCE]? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :FRTD:TYPE {85|91}{,<@<ch_list>}}
    :FRTD:TYPE? [{<@<ch_list>}]
    :FRTD:RESistance[:REfERENCE] <reference>{,<@<ch_list>}}
    :FRTD:RESistance[:REfERENCE]? [{<@<ch_list>}]

[SENSe:]TEMPerature:TRANSDUCER
    :THERmistor:TYPE {2252|5000|10000}{,<@<ch_list>}}
    :THERmistor:TYPE? [{<@<ch_list>}]

[SENSe:]
    TEMPerature:NPLC {0.02|0.2|1|2|10|20|100|200|MIN|MAX}{,<@<ch_list>}}
    TEMPerature:NPLC? [{<@<ch_list>}|MIN|MAX]}

```

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Voltage Configuration Commands

(see page 223 in the User's Guide)

```

S CONFIGure
    :VOLTage:DC [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF}},] (@<scan_list>)
CONFIGure? [(@<ch_list>)]

[SENSe:]
    VOLTage:DC:RANGe [{<range>|MIN|MAX}[, (@<ch_list>)]]
    VOLTage:DC:RANGe? [({@<ch_list>})|MIN|MAX]]
    VOLTage:DC:RANGe:AUTO {OFF|ON}[, (@<ch_list>)]
    VOLTage:DC:RANGe:AUTO? [(@<ch_list>)]

[SENSe:]
    VOLTage:DC:RESolution {<resolution>|MIN|MAX}[, (@<ch_list>)]
    VOLTage:DC:RESolution? [({@<ch_list>})|MIN|MAX]]

[SENSe:]
    VOLTage:DC:APERTure {<time>|MIN|MAX}[, (@<ch_list>)]
    VOLTage:DC:APERTure? [({@<ch_list>})|MIN|MAX]]

[SENSe:]
    VOLTage:DC:NPLC {0.02|0.2|1|2|10|20|100|200|MIN|MAX}[, (@<ch_list>)]
    VOLTage:DC:NPLC? [({@<ch_list>})|MIN|MAX]]

INPut
    :IMPedance:AUTO {OFF|ON}[, (@<ch_list>)]
    :IMPedance:AUTO? [(@<ch_list>)]

[SENSe:]
    ZERO:AUTO {OFF|ONCE|ON}[, (@<ch_list>)]
    ZERO:AUTO? [(@<ch_list>)]

S CONFIGure
    :VOLTage:AC [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF}},] (@<scan_list>)
CONFIGure? [(@<ch_list>)]

[SENSe:]
    VOLTage:AC:RANGe [{<range>|MIN|MAX}[, (@<ch_list>)]
    VOLTage:AC:RANGe? [({@<ch_list>})|MIN|MAX]]
    VOLTage:AC:RANGe:AUTO {OFF|ON}[, (@<ch_list>)]
    VOLTage:AC:RANGe:AUTO? [(@<ch_list>)]

[SENSe:]
    VOLTage:AC:BANDwidth {3|20|200|MIN|MAX}[, (@<ch_list>)]
    VOLTage:AC:BANDwidth? [({@<ch_list>})|MIN|MAX]]
  
```

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Resistance Configuration Commands

(see page 224 in the User's Guide)

```

S CONFIGure
:RESistance [{<range>|AUTO|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF]], ] (@<scan_list>)
CONFIGure? [{@<ch_list>}]

[SENSe:]
RESistance:RANge {<range>|MIN|MAX}[, (@<ch_list>)]
RESistance:RANge? [{(@<ch_list>)|MIN|MAX}]
RESistance:RANge:AUTO {OFF|ON}[, (@<ch_list>)]
RESistance:RANge:AUTO? [{@<ch_list>}]

[SENSe:]
RESistance:RESolution {<resolution>|MIN|MAX}[, (@<ch_list>)]
RESistance:RESolution? [{(@<ch_list>)|MIN|MAX}]
RESistance:APERTure {<time>|MIN|MAX}[, (@<ch_list>)]
RESistance:APERTure? [{(@<ch_list>)|MIN|MAX}]
RESistance:NPLC {0.02|0.2|1|2|10|20|100|200|MIN|MAX}[, (@<ch_list>)]
RESistance:NPLC? [{(@<ch_list>)|MIN|MAX}]

[SENSe:]
RESistance:OCOMpensated {OFF|ON}[, (@<ch_list>)]
RESistance:OCOMpensated? [{@<ch_list>}]

S CONFIGure
:FRESistance [{<range>|AUTO|MIN|MAX|DEF}
[, <resolution>|MIN|MAX|DEF]], ] (@<scan_list>)
CONFIGure? [{@<ch_list>}]

[SENSe:]
FRESistance:RANge {<range>|MIN|MAX}[, (@<ch_list>)]
FRESistance:RANge? [{(@<ch_list>)|MIN|MAX}]
FRESistance:RANge:AUTO {OFF|ON}[, (@<ch_list>)]
FRESistance:RANge:AUTO? [{@<ch_list>}]

[SENSe:]
FRESistance:RESolution {<resolution>|MIN|MAX}[, (@<ch_list>)]
FRESistance:RESolution? [{(@<ch_list>)|MIN|MAX}]
FRESistance:APERTure {<time>|MIN|MAX}[, (@<ch_list>)]
FRESistance:APERTure? [{(@<ch_list>)|MIN|MAX}]
FRESistance:NPLC {0.02|0.2|1|2|10|20|100|200|MIN|MAX}[, (@<ch_list>)]
FRESistance:NPLC? [{(@<ch_list>)|MIN|MAX}]

[SENSe:]
FRESistance:OCOMpensated {OFF|ON}[, (@<ch_list>)]
FRESistance:OCOMpensated? [{@<ch_list>}]

```

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Current Configuration Commands

(see page 224 in the User's Guide)

Valid only on channels 21 and 22 on the 34901A multiplexer module.

```

S CONFIGure
    :CURRENT:DC [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF]],] (@<scan_list>)
CONFIGure? [{(@<ch_list>)]

[SENSe:]
CURRENT:DC:RANge {<range>|MIN|MAX}{, (@<ch_list>)}
CURRENT:DC:RANge? [{(@<ch_list>)|MIN|MAX}]
CURRENT:DC:RANge:AUTO {OFF|ON}{, (@<ch_list>)}
CURRENT:DC:RANge:AUTO? [{(@<ch_list>)}]

[SENSe:]
CURRENT:DC:RESolution {<resolution>|MIN|MAX}{, (@<ch_list>)}
CURRENT:DC:RESolution? [{(@<ch_list>)|MIN|MAX}]

[SENSe:]
CURRENT:DC:APERture {<time>|MIN|MAX}{, (@<ch_list>)}
CURRENT:DC:APERture? [{(@<ch_list>)|MIN|MAX}]

[SENSe:]
CURRENT:DC:NPLC {0.02|0.2|1|2|10|20|100|200|MIN|MAX}{, (@<ch_list>)}
CURRENT:DC:NPLC? [{(@<ch_list>)|MIN|MAX}]

S CONFIGure
    :CURRENT:AC [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF]],] (@<scan_list>)
CONFIGure? [{(@<ch_list>)]

[SENSe:]
CURRENT:AC:RANge {<range>|MIN|MAX}{, (@<ch_list>)}
CURRENT:AC:RANge? [{(@<ch_list>)|MIN|MAX}]
CURRENT:AC:RANge:AUTO {OFF|ON}{, (@<ch_list>)}
CURRENT:AC:RANge:AUTO? [{(@<ch_list>)}]

[SENSe:]
CURRENT:AC:BANDwidth {3|20|200|MIN|MAX}{, (@<ch_list>)}
CURRENT:AC:BANDwidth? [{(@<ch_list>)|MIN|MAX}]

```

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Frequency and Period Configuration Commands

(see page 214 in the User's Guide)

```

S CONFIGure
    :FREQuency [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF]],] (@<scan_list>)
CONFIGure? [{(@<ch_list>)]

[SENSe:]
    FREQuency:VOLTage:RANGe {<range>|MIN|MAX}[, (@<ch_list>)]
    FREQuency:VOLTage:RANGe? [{(@<ch_list>)|MIN|MAX}]
    FREQuency:VOLTage:RANGe:AUTO {OFF|ON}[, (@<ch_list>)]
    FREQuency:VOLTage:RANGe:AUTO? [{(@<ch_list>)]

[SENSe:]
    FREQuency:APERture {0.01|0.1|1|MIN|MAX}[, (@<ch_list>)]
    FREQuency:APERture? [{(@<ch_list>)|MIN|MAX}]

[SENSe:]
    FREQuency:RANGe:LOWer {3|20|200|MIN|MAX}[, (@<ch_list>)]
    FREQuency:RANGe:LOWer? [{(@<ch_list>)|MIN|MAX}]

S CONFIGure
    :PERiod [{<range>|AUTO|MIN|MAX|DEF}
    [, <resolution>|MIN|MAX|DEF]],] (@<scan_list>)
CONFIGure? [{(@<ch_list>)]

[SENSe:]
    PERiod:VOLTage:RANGe {<range>|MIN|MAX}[, (@<ch_list>)]
    PERiod:VOLTage:RANGe? [{(@<ch_list>)|MIN|MAX}]
    PERiod:VOLTage:RANGe:AUTO {OFF|ON}[, (@<ch_list>)]
    PERiod:VOLTage:RANGe:AUTO? [{(@<ch_list>)]

[SENSe:]
    PERiod:APERture {0.01|0.1|1|MIN|MAX}[, (@<ch_list>)]
    PERiod:APERture? [{(@<ch_list>)|MIN|MAX}]

```

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Mx+B Scaling Commands

(see page 244 in the User's Guide)

```
CALCulate
:SCALE:GAIN <gain>[, (@<ch_list>)]
:SCALE:GAIN? [(@<ch_list>)]
:SCALE:OFFSET <offset>[, (@<ch_list>)]
:SCALE:OFFSET? [(@<ch_list>)]
:SCALE:UNIT <quoted_string>[, (@<ch_list>)]
:SCALE:UNIT? [(@<ch_list>)]

CALCulate:SCALE:OFFSET:NULL [(@<ch_list>)]

CALCulate
:SCALE:STATE {OFF|ON}[, (@<ch_list>)]
:SCALE:STATE? [(@<ch_list>)]
```

Alarm Limit Commands

(see page 247 in the User's Guide)

```
OUTPut
:ALARm[1|2|3|4]:SOURce (@<ch_list>)
:ALARm[1|2|3|4]:SOURce?

CALCulate
:LIMit:UPPer <hi_limit>[, (@<ch_list>)]
:LIMit:UPPer? [(@<ch_list>)]
:LIMit:UPPer:STATE {OFF|ON}[, (@<ch_list>)]
:LIMit:UPPer:STATE? [(@<ch_list>)]

CALCulate
:LIMit:LOWer <lo_limit>[, (@<ch_list>)]
:LIMit:LOWer? [(@<ch_list>)]
:LIMit:LOWer:STATE {OFF|ON}[, (@<ch_list>)]
:LIMit:LOWer:STATE? [(@<ch_list>)]

SYSTem:ALARm?

G OUTPut
:ALARm:MODE (LATCh|TRACK)
:ALARm:MODE?
:ALARm:SLOPe (NEGative|POSitive)
:ALARm:SLOPe?

OUTPut
:ALARm[1|2|3|4]:CLear
:ALARm:CLear:ALL

STATus
:ALARm:CONDition?
:ALARm:ENABle <enable_value>
:ALARm:ENABle?
:ALARm[:EVENT]?



|           |           |           |       |       |
|-----------|-----------|-----------|-------|-------|
| Ch 01     | Ch 02     | Ch 03     | Ch 04 | Ch 05 |
| DIO (LSB) | DIO (MSB) | Totalizer | DAC   | DAC   |



CALCulate
:COMParE:TYPE {EQUAL|NEQual}[, (@<ch_list>)]
:COMParE:TYPE? [(@<ch_list>)]
:COMParE:DATA <data>[, (@<ch_list>)]
:COMParE:DATA? [(@<ch_list>)]
:COMParE:MASK <mask>[, (@<ch_list>)]
:COMParE:MASK? [(@<ch_list>)]
:COMParE:STATE {OFF|ON}[, (@<ch_list>)]
:COMParE:STATE? [(@<ch_list>)]
```

G This command applies to all channels in the instrument (Global setting).
Default parameters are shown in **bold**.

Digital Input Commands

(see page 255 in the User's Guide)

Ch 01	Ch 02	Ch 03	Ch 04	Ch 05
DIO (LSB)	DIO (MSB)	Totalizer	DAC	DAC

S CONFIGure:DIGital:BYTE (@<scan_list>
CONFIGure? [{@<ch_list>}]

[SENSe:]DIGital:DATA:{**BYTE**|WORD}? [{@<ch_list>}]

Totalizer Commands

(see page 256 in the User's Guide)

Ch 01	Ch 02	Ch 03	Ch 04	Ch 05
DIO (LSB)	DIO (MSB)	Totalizer	DAC	DAC

S CONFIGure:TOTalize {**READ**|RRESet} , (@<scan_list>
CONFIGure? [{@<ch_list>}]

[SENSe:]
TOTalize:TYPE {**READ**|RRESet} [, (@<ch_list>)]
TOTalize:TYPE? [{@<ch_list>}]

[SENSe:]
TOTalize:SLOPe {**NEGative**|**POSitive**} [, (@<ch_list>)]
TOTalize:SLOPe? [{@<ch_list>}]

[SENSe:]TOTalize:CLear:IMMediate [{@<ch_list>}]

[SENSe:]TOTalize:DATA? [{@<ch_list>}]

Digital Output Commands

(see page 258 in the User's Guide)

Ch 01	Ch 02	Ch 03	Ch 04	Ch 05
DIO (LSB)	DIO (MSB)	Totalizer	DAC	DAC

SOURCE
:DIGital:DATA[:{**BYTE**|WORD}] <data> , (@<ch_list>)
:DIGital:DATA[:{**BYTE**|WORD}]? (@<ch_list>)

SOURCE:DIGital:STate? (@<ch_list>)

DAC Output Commands

(see page 258 in the User's Guide)

Ch 01	Ch 02	Ch 03	Ch 04	Ch 05
DIO (LSB)	DIO (MSB)	Totalizer	DAC	DAC

SOURCE
:VOLTage <voltage> , (@<ch_list>)
:VOLTage? (@<ch_list>)

S This command redefines the scan list when executed.
Default parameters are shown in **bold**.

Switch Control Commands

(see page 259 in the User's Guide)

ROUTe

:CLOSe (@<ch_list>)
:CLOSe:EXCLUsive (@<ch_list>)
:CLOSe? (@<ch_list>)

ROUTe

:OPeN (@<ch_list>)
:OPeN? (@<ch_list>)

ROUTe:DONe?

SYSTem:CPON {100|200|300|ALL}

Scan Triggering Commands

(see page 228 in the User's Guide)

G TRIGger
:SOURce {BUS|**IMMediate**|EXTeRnal|ALARm1|ALARm2|ALARm3|ALARm4|TImeR}
:SOURce?

G TRIGger
:TImeR (<seconds>|**MIN**|MAX)
:TImeR?

G TRIGger
:COUNt (<count>|**MIN**|MAX|INFIinity)
:COUNt?

*TRG

INITiate

READ?

State Storage Commands

(see page 261 in the User's Guide)

*SAV {0|1|2|3|4|5}
*RCL {0|1|2|3|4|5}

MEMory:STATe
:NAME {1|2|3|4|5} [, <name>]
:NAME? {1|2|3|4|5}

MEMory:STATe:DELeTe {0|1|2|3|4|5}

MEMory:STATe
:RECall:AUTO {OFF|**ON**}
:RECall:AUTO?

MEMory:STATe:VALId? {0|1|2|3|4|5}

MEMory:NSTATes?

G This command applies to all channels in the instrument (Global setting).
Default parameters are shown in **bold**.

System-Related Commands

(see page 264 in the User's Guide)

```
SYSTem
:DATE <yyyy> , <mm> , <dd>
:DATE?
:TIME <hh> , <mm> , <ss.sss>
:TIME?

FORMat
:READing:TIME:TYPE {ABSolute|RELative}
:READing:TIME:TYPE?

*IDN?

SYSTem:CTYPE? {100|200|300}

DIAGnostic
:POKE:SLOT:DATA {100|200|300} , <quoted_string>
:PEEK:SLOT:DATA? {100|200|300}

DISPlay {OFF|ON}
DISPlay?

DISPlay
:TEXT <quoted_string>
:TEXT?
:TEXT:CLEar

*RST

SYSTem:PRESet

SYSTem:CPON {100|200|300|ALL}

SYSTem:ERRor?

SYSTem:ALARm?

SYSTem:VERSion?

*TST?
```

Interface Configuration Commands

(see page 269 in the User's Guide)

```
SYSTem:INTerface {GPIB|RS232}

SYSTem:LOCal

SYSTem:REMOte

SYSTem:RWLock
```

Default parameters are shown in **bold**

Status System Commands

(see page 286 in the User's Guide)

```
*STB?
*SRE <enable_value>

*SRE?

STATus
:QUESTionable:CONDition?
:QUESTionable[:EVENT]?
:QUESTionable:ENABle <enable_value>
:QUESTionable:ENABle?

*ESR?
*ESE <enable_value>
*ESE?

STATus
:ALARm:CONDition?
:ALARm[:EVENT]?
:ALARm:ENABle <enable_value>
:ALARm:ENABle?

STATus
:OPERation:CONDition?
:OPERation[:EVENT]?
:OPERation:ENABle <enable_value>
:OPERation:ENABle?

DATA:POINTs
:EVENT:THReshold <num_rdgs>
:EVENT:THReshold?

*CLS

*PSC {0|1}
*PSC?

*OPC
```

Calibration Commands

(see page 292 in the User's Guide)

```
CALibration?

CALibration:COUNT?

CALibration
:SECure:CODE <new_code>
:SECure:STATE {OFF|ON}, <code>
:SECure:STATE?

CALibration
:STRing <quoted_string>
:STRing?

CALibration
:VALue <value>
:VALue?
```

Service-Related Commands

(see page 294 in the User's Guide)

```
INSTRument
: DMM {OFF|ON}
: DMM?
: DMM:INSTalled?

DIAGnostic
: DMM:CYCLes?
: DMM:CYCLes:CLear {1|2|3}

DIAGnostic
: RELay:CYCLes? [{@<ch_list>}]
: RELay:CYCLes:CLear [{@<ch_list>}]

*RST

SYSTem:PRESet

SYSTem:CPON {100|200|300|ALL}

SYSTem:VERSion?

*TST?
```

IEEE 488.2 Common Commands

```
*CLS

*ESR?
*ESE <enable_value>
*ESE?

*IDN?

*OPC

*OPC?

*PSC {0|1}
*PSC?

*RST

*SAV {0|1|2|3|4|5}
*RCL {0|1|2|3|4|5}

*STB?
*SRE <enable_value>
*SRE?


*TRG

*TST?
```

*Default parameters are shown in **bold**.*


34901A 20-Channel Multiplexer

(see page 164 in the User's Guide)

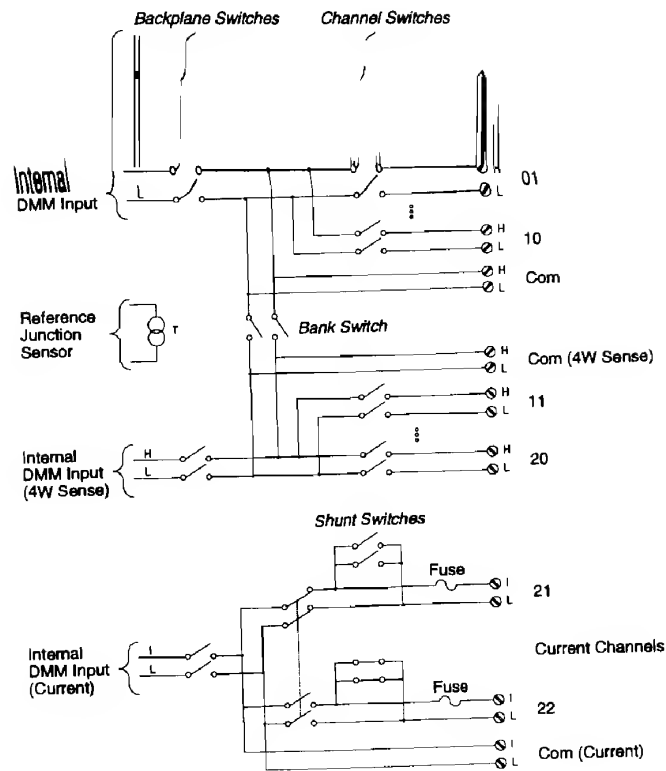


34902A 16-Channel Multiplexer

(see page 166 in the User's Guide)

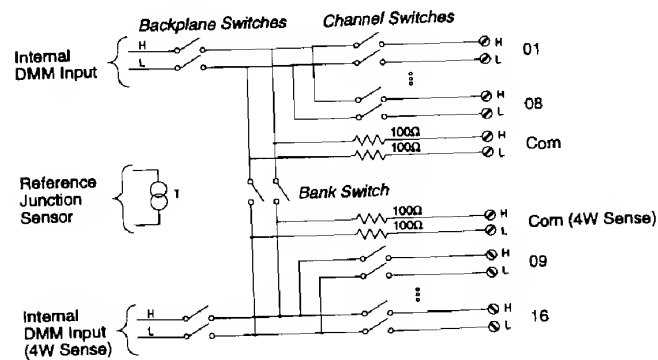


34903A 20-Channel Actuator

(see page 168 in the User's Guide)




34904A 4x8 Matrix

(see page 170 in the User's Guide)

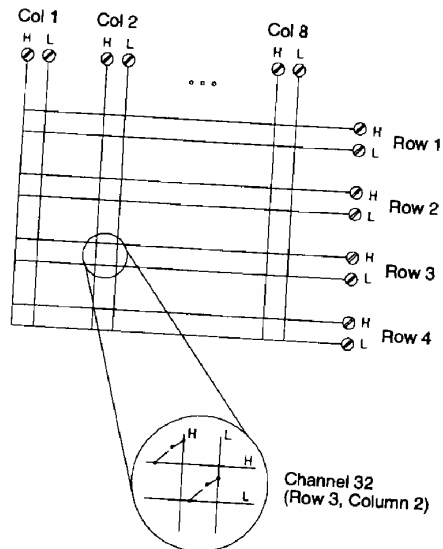


34905A/6A Dual 4-Channel RF Multiplexers

(see page 172 in the User's Guide)

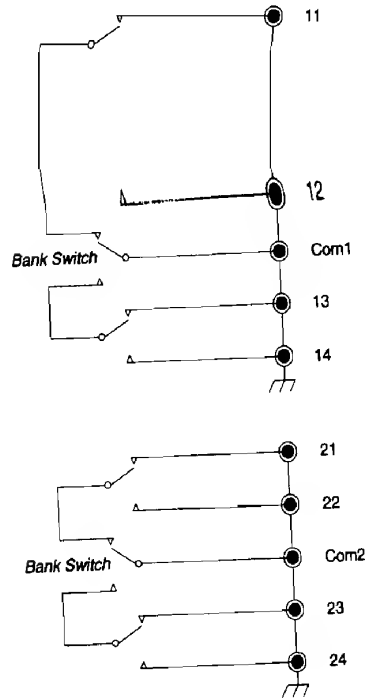





34908A 40-Channel Single-Ended Multiplexer

(see page 174 in the User's Guide)

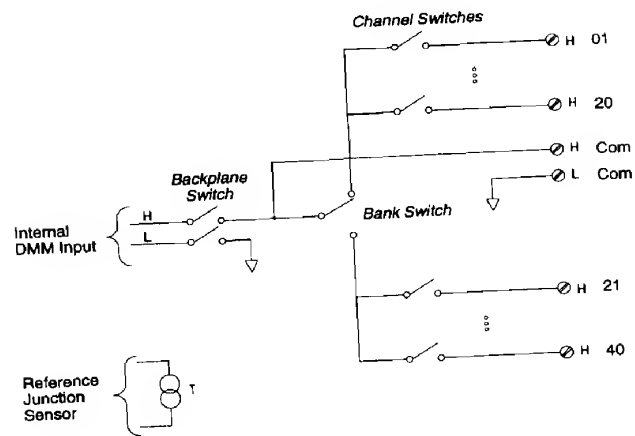

34907A Multifunction Module

(see page 176 in the User's Guide)

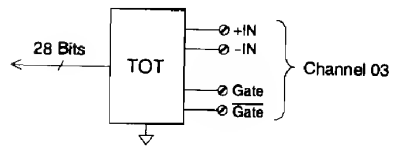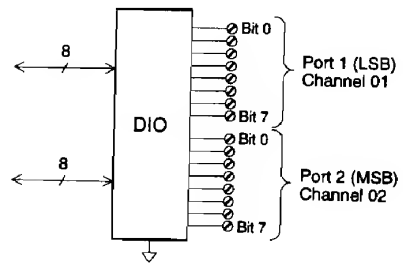

Factory Reset State

The table below shows the state of the instrument after a FACTORY RESET from the *Sto/Rcl* menu or *RST command from the remote interface.

Measurement Configuration	Factory Reset State
Function	DC Volts
Range	Autorange
Resolution	5½ digits
Integration Time	1 PLC
Input Resistance	10 M Ω (fixed for all DCV ranges)
Channel Delay	Automatic Delay
Totalizer Reset Mode	Count Not Reset When Read
Totalizer Edge Detect	Rising Edge
Scanning Operations	Factory Reset State
Scan List	Empty
Reading Memory	All Readings are Cleared
Min, Max, and Average	All Statistical Data is Cleared
Scan Interval Source	Immediate
Scan Interval	Front Panel = 10 Seconds Remote = Immediate
Scan Count	Front Panel = Continuous Remote = 1 Scan Sweep
Scan Reading Format	Reading Only (No Units, Channel, Time)
Monitor in Progress	Stopped
Mx+B Scaling	Factory Reset State
Gain Factor ("M")	1
Scale Factor ("B")	0
Scale Label	Vdc
Alarm Limits	Factory Reset State
Alarm Queue	Not Cleared
Alarm State	Off
HI and LO Alarm Limits	0
Alarm Output	Alarm 1
Alarm Output Configuration	Latched Mode
Alarm Output State	Output Lines are Cleared
Alarm Output Slope	Fail = Low
Module Hardware	Factory Reset State
34901A, 34902A, 34908A	Reset: All Channels Open
34903A, 34904A	Reset: All Channels Open
34905A, 34906A	Reset: Channels s11 and s21 Selected
34907A	Reset: Both DIO Ports = Input, Count = 0, Both DACs = 0 Vdc
System-Related Operations	Factory Reset State
Display State	On
Error Queue	Errors Not Cleared
Stored States	No Change





Agilent Technologies
Innovating the HP Way

*As of November 1, 1999, Agilent Technologies is a subsidiary of Hewlett-Packard Company. This is a change in name only. All product features and functionality remain as described in the enclosed documentation. For more information, refer to the Agilent Technologies web site at **www.agilent.com**.*

This package contains the following:

- Agilent 34970A User's Guide
- Agilent 34970A Quick Reference
- Agilent 34970A Service Guide

Agilent Technologies, Inc.
Printed in U.S.A.
Edition 3
November 1999 E1199



34970-90100